



Real-Time Water Quality Deployment Report

Rattling Brook Network

February 21, 2023 to March 28, 2023



Government of Newfoundland & Labrador
Department of Environment and Climate Change
Water Resources Management Division
St. John's, NL, A1B 4J6 Canada

General

- Department of Environment and Climate Change staff monitor the real-time web pages consistently.
- Hydrometric data included in this report is provisional and used only for illustrative purposes. Corrected and finalized data may be retrieved from the Water Survey of Canada website (https://wateroffice.ec.gc.ca/index_e.html)*.

Maintenance and Calibration of Instrument

- As part of the Quality Assurance and Quality Control protocol (QAQC), an assessment of the reliability of data recorded by an instrument is made at the beginning and end of the deployment period. The procedure is based on the approach used by the United States Geological Survey.
 - Upon deployment, a QA/QC Sonde is temporarily deployed *in situ*, adjacent to the Field Sonde. Depending on the degree of difference between each parameter from the Field and QAQC sondes, a qualitative rank is assigned (See Table 1). The possible ranks, from most to least desirable, are: Excellent, Good, Fair, Marginal, and Poor. A grab sample is also taken for additional confirmation of conditions at deployment and to allow for future modelling studies.
 - At the end of a deployment period, a freshly cleaned and calibrated QAQC Sonde is placed *in situ*, adjacent to the Field Sonde. Values are compared between all parameters and differences are ranked for placement in Table 1.

Table 1: Qualitative QAQC Ranking


Station	Date	Action	Comparison Ranking				
			Temperature	pH	Conductivity	Dissolved Oxygen	Turbidity
Rattling Brook Big Pond	January 26	Deployment	Fair	Good	Marginal	Good	Excellent
	March 28	Ongoing	N/A	N/A	N/A	N/A	N/A
Rattling Brook below Bridge	February 21	Deployment	Excellent	Excellent	Good	Fair	Poor
	March 28	Removal	Excellent	Fair	Good	Excellent	Poor
Rattling Brook below Plant Discharge	February 21	Deployment	Good	Excellent	Excellent	Excellent	Fair
	March 28	Removal	Good	Good	Fair	Fair	Excellent

- The VALE weather station in Long Harbour installation was completed in February 2023. Deployment reports will utilize that station’s data from this day forward.
- On February 21st when visiting Rattling Brook, the weather at the time was heavy rain which prompted Below Bridge Turbidity ranking of ‘Poor’ on deployment of the field sonde. Field sonde measured 22.0 NTU while the QA/QC sonde measured 10.0 NTU and the grab sample measurement was 11.0 NTU.

- Data Interpretation

Temperature

Water Temperature is a major factor used to describe water quality. Temperature has major implications on both the ecology and chemistry of a water body, governing processes such as the metabolic rate of aquatic plants and animals and the degree of dissolved oxygen saturation.

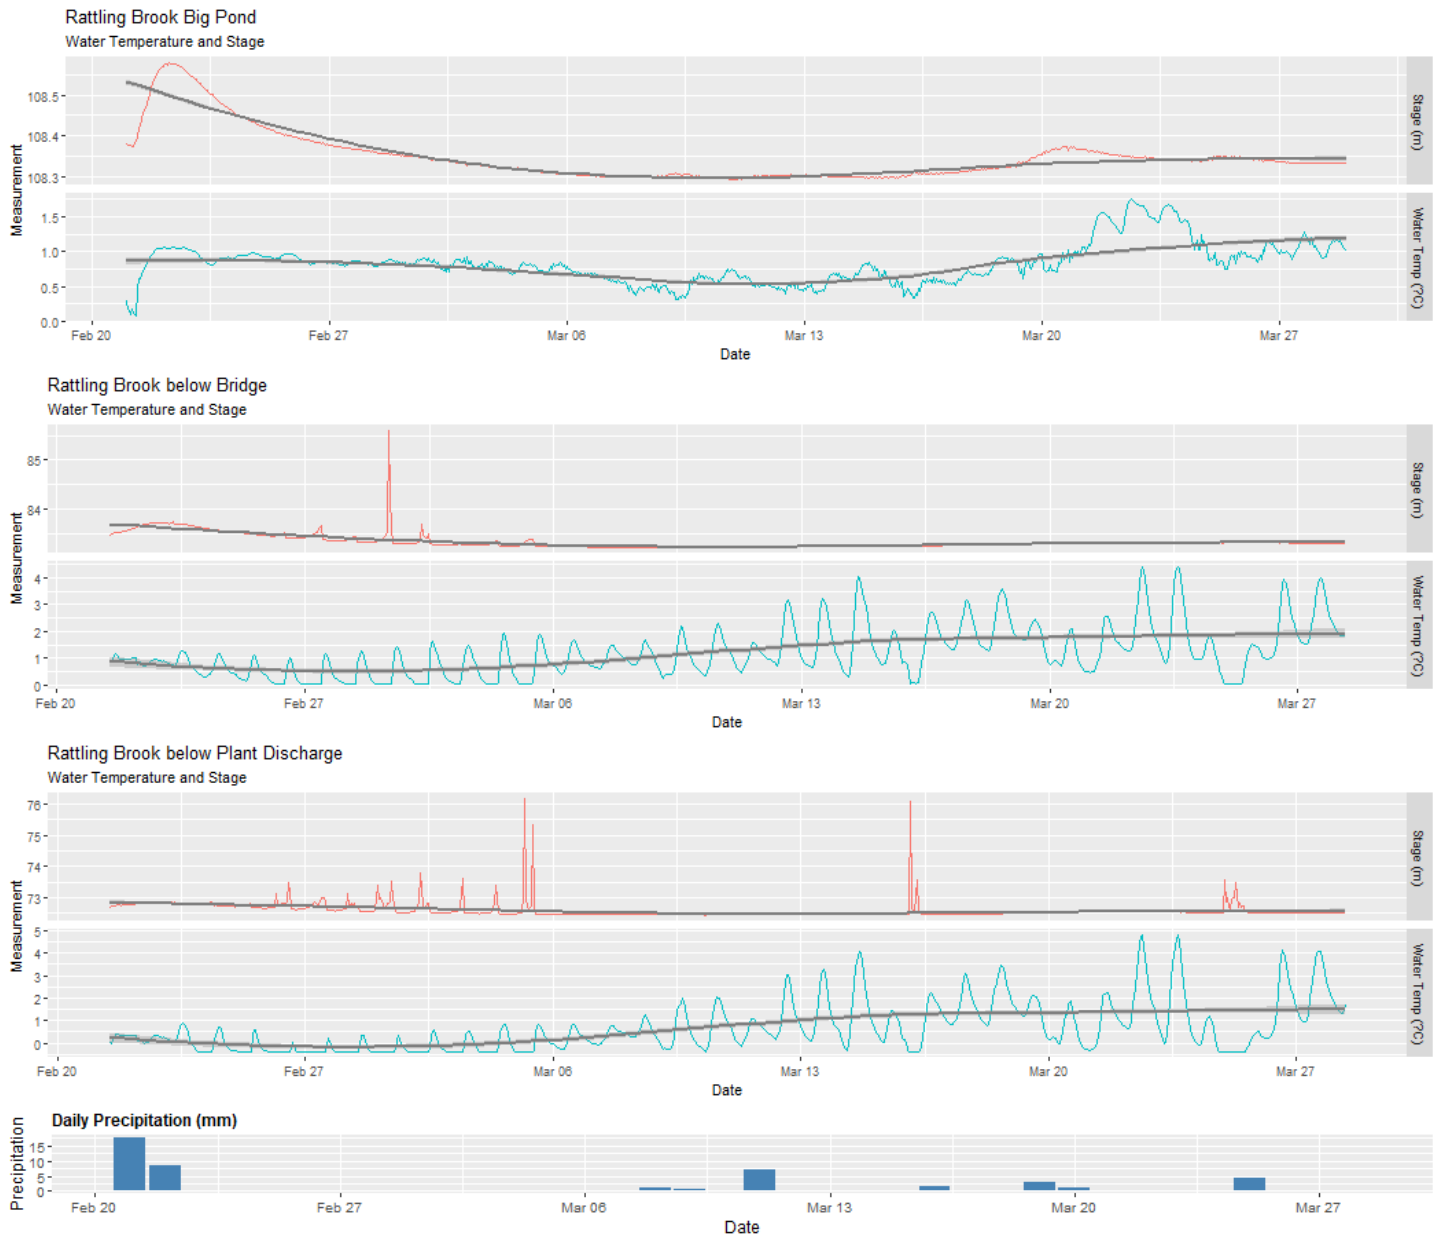


- Trend lines show water temperatures slowly increasing at all three stations.

*All hydrometric data is provisional and is subject to correction. Please consult Water survey of Canada for finalized data and interpretation.

pH

pH is used to give an indication of the acidity or basicity of a solution. A pH of 7 denotes a neutral solution while lower values are acidic and higher values are basic. Technically, the pH of a solution indicates the availability of protons to react with molecules dissolved in water. Such reactions can affect how molecules function chemically and metabolically.

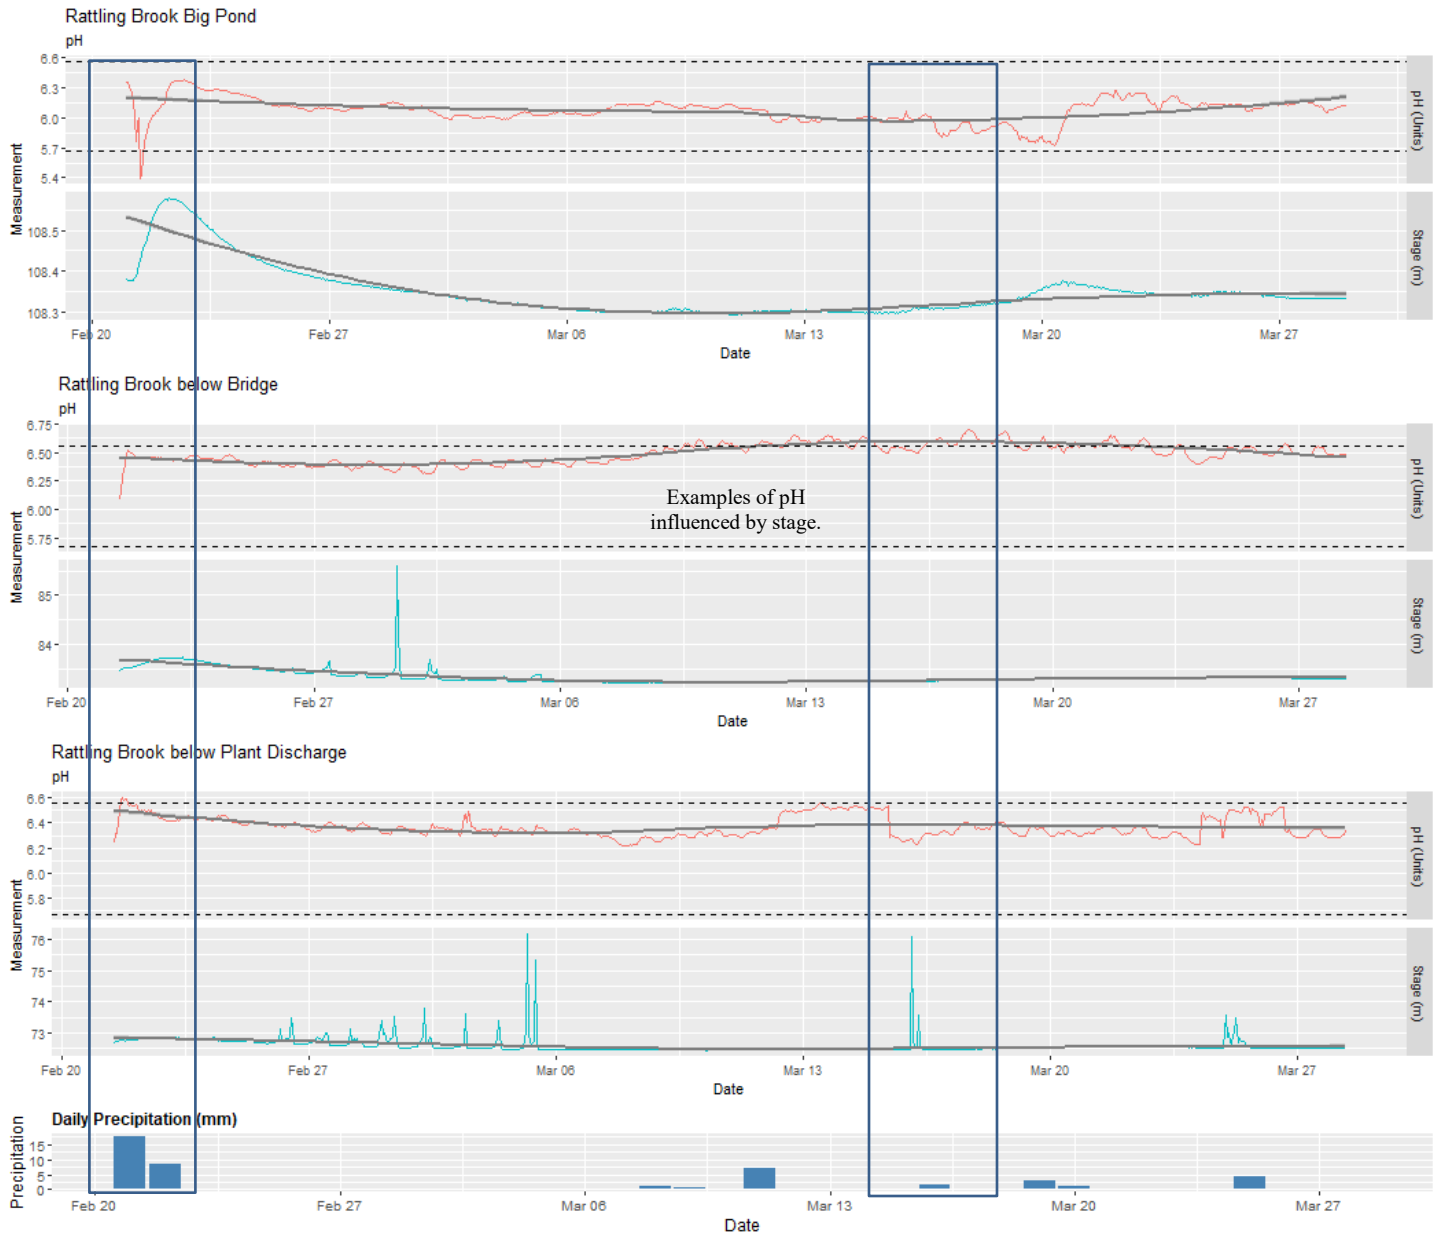


Station	Max	Min	Median	Mean
Big Pond	6.38	5.39	6.09	6.07
Below Bridge	6.70	6.08	6.49	6.49
Below Plant Discharge	6.60	6.22	6.35	6.37

- pH values were consistent with the majority of values within the site-specific guidelines (5.67-6.56 pH Units) except at below Bridge.

*All hydrometric data is provisional and is subject to correction. Please consult Water survey of Canada for finalized data and interpretation.


Specific Conductivity

Conductivity relates to the ease of passing an electric charge – or resistance – through a solution. Conductivity is highly influenced by the concentration of dissolved ions in solution: distilled water has zero conductivity (infinite resistance) while salty solutions have high conductivity (low resistance). Specific Conductivity is corrected to 25°C to allow comparison across variable temperatures.

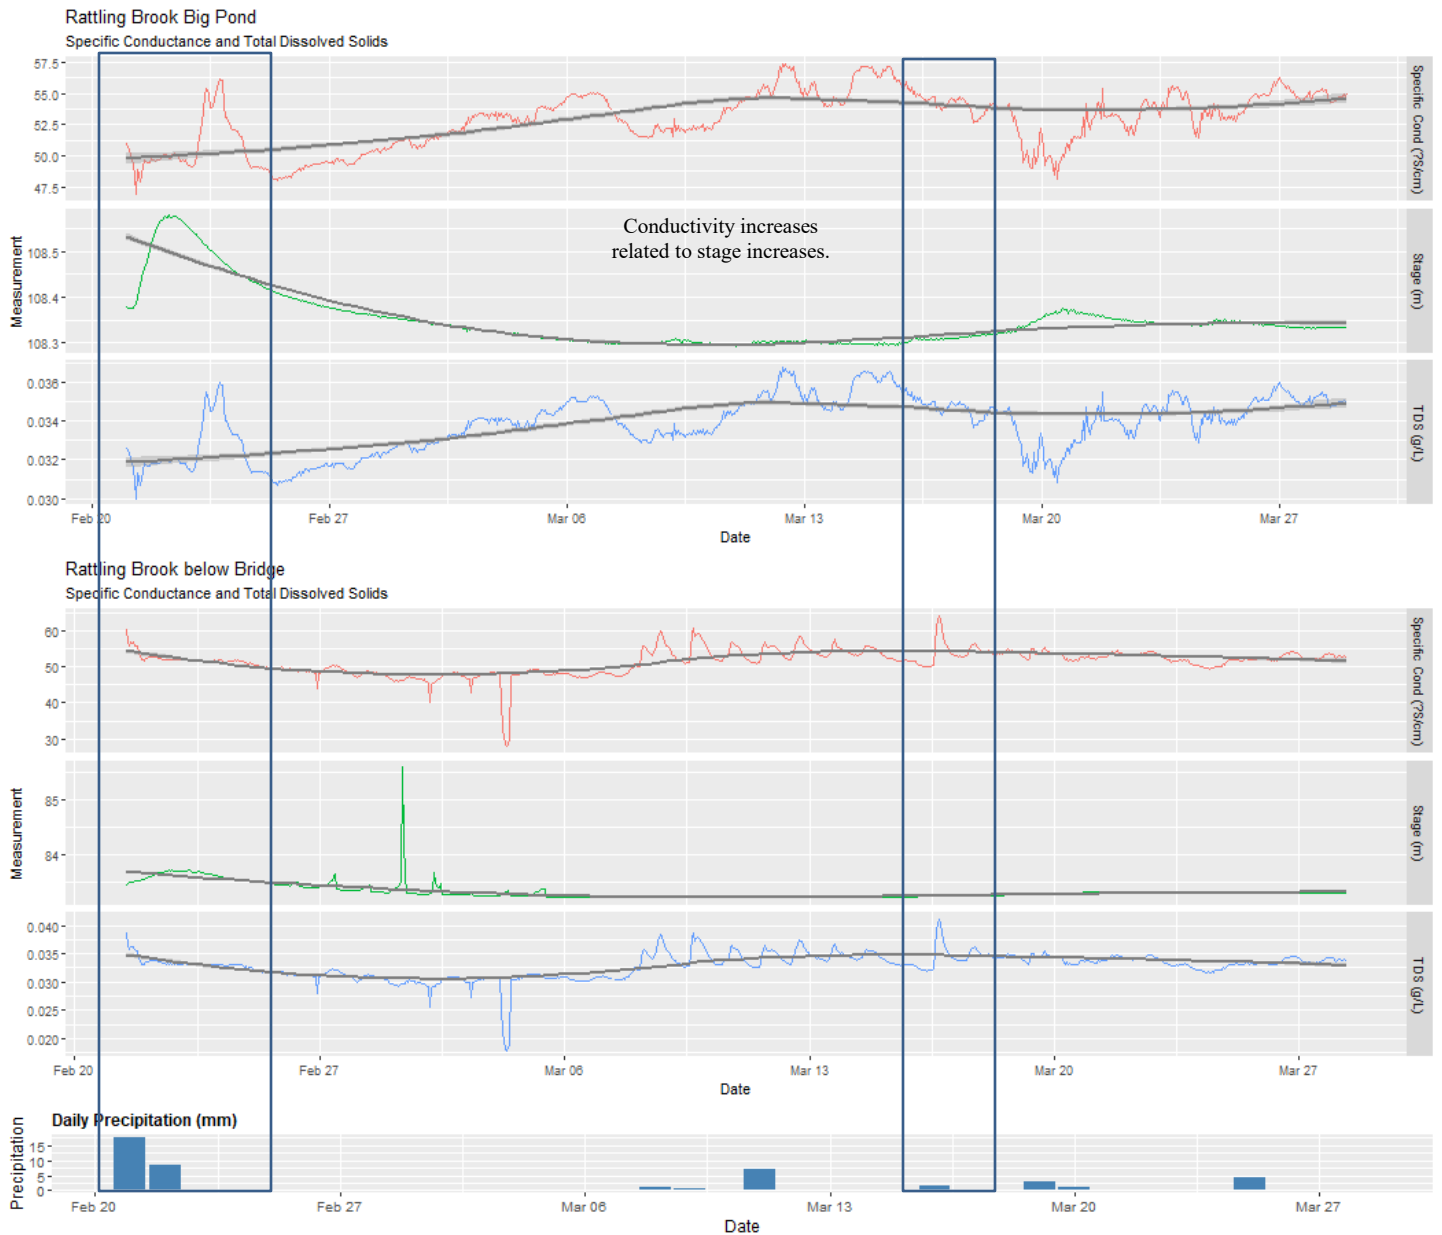

*All hydrometric data is provisional and is subject to correction. Please consult Water survey of Canada for finalized data and interpretation.

Rattling Brook Network, Long Harbour, Newfoundland and Labrador

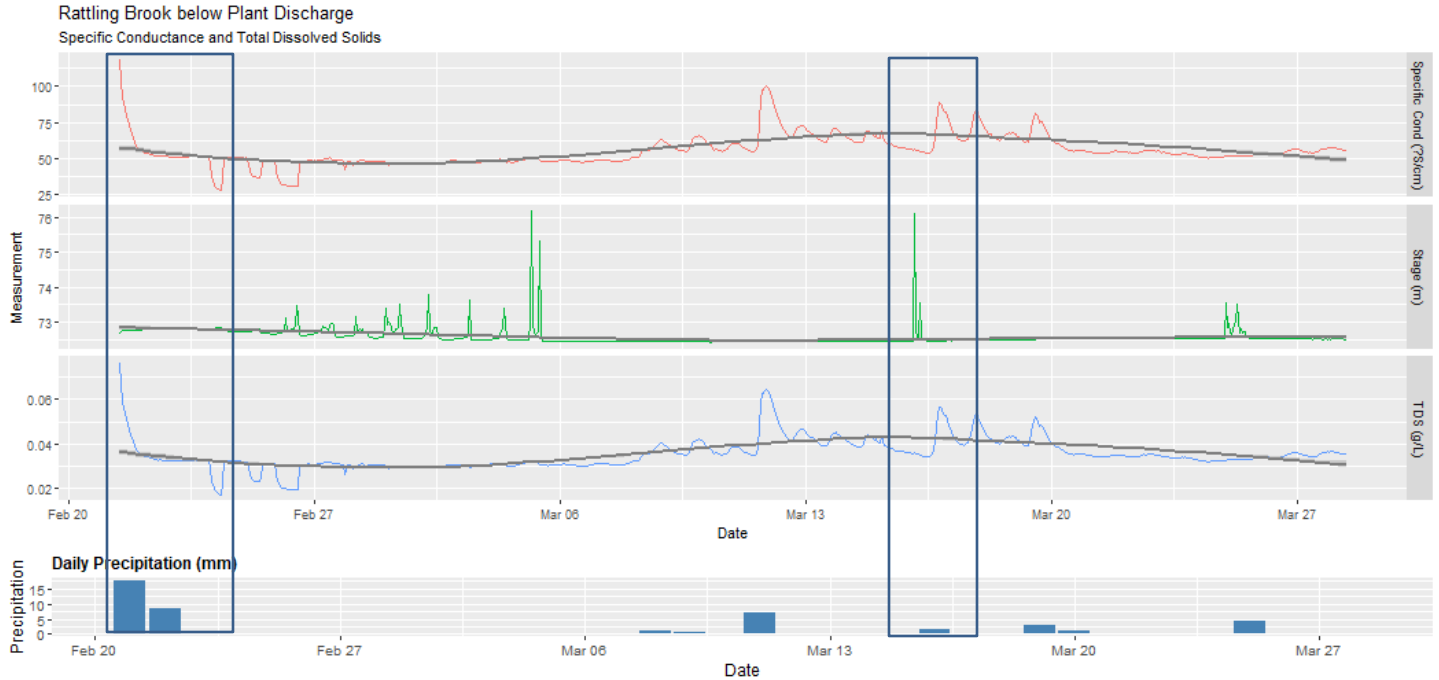


Station	Max	Min	Median	Mean
Big Pond	57.4	46.9	53.2	52.9
Below Bridge	64.2	27.9	51.9	51.4
Below Plant Discharge	118.9	27.4	53.5	55.4

- Specific conductivity was relatively stable at all stations with most peaks occurring during precipitation events.

*All hydrometric data is provisional and is subject to correction. Please consult Water survey of Canada for finalized data and interpretation.


Dissolved Oxygen

Dissolved oxygen is a metabolic requirement of aquatic plants and animals. The concentration of oxygen in water depends on many factors, especially temperature – the saturation of oxygen in water is inversely proportional to water temperature. Oxygen concentrations also tend to be higher in flowing water compared to still, lake environments. Low oxygen concentrations can give an indication of excessive decomposition of organic matter or oxidation reactions.

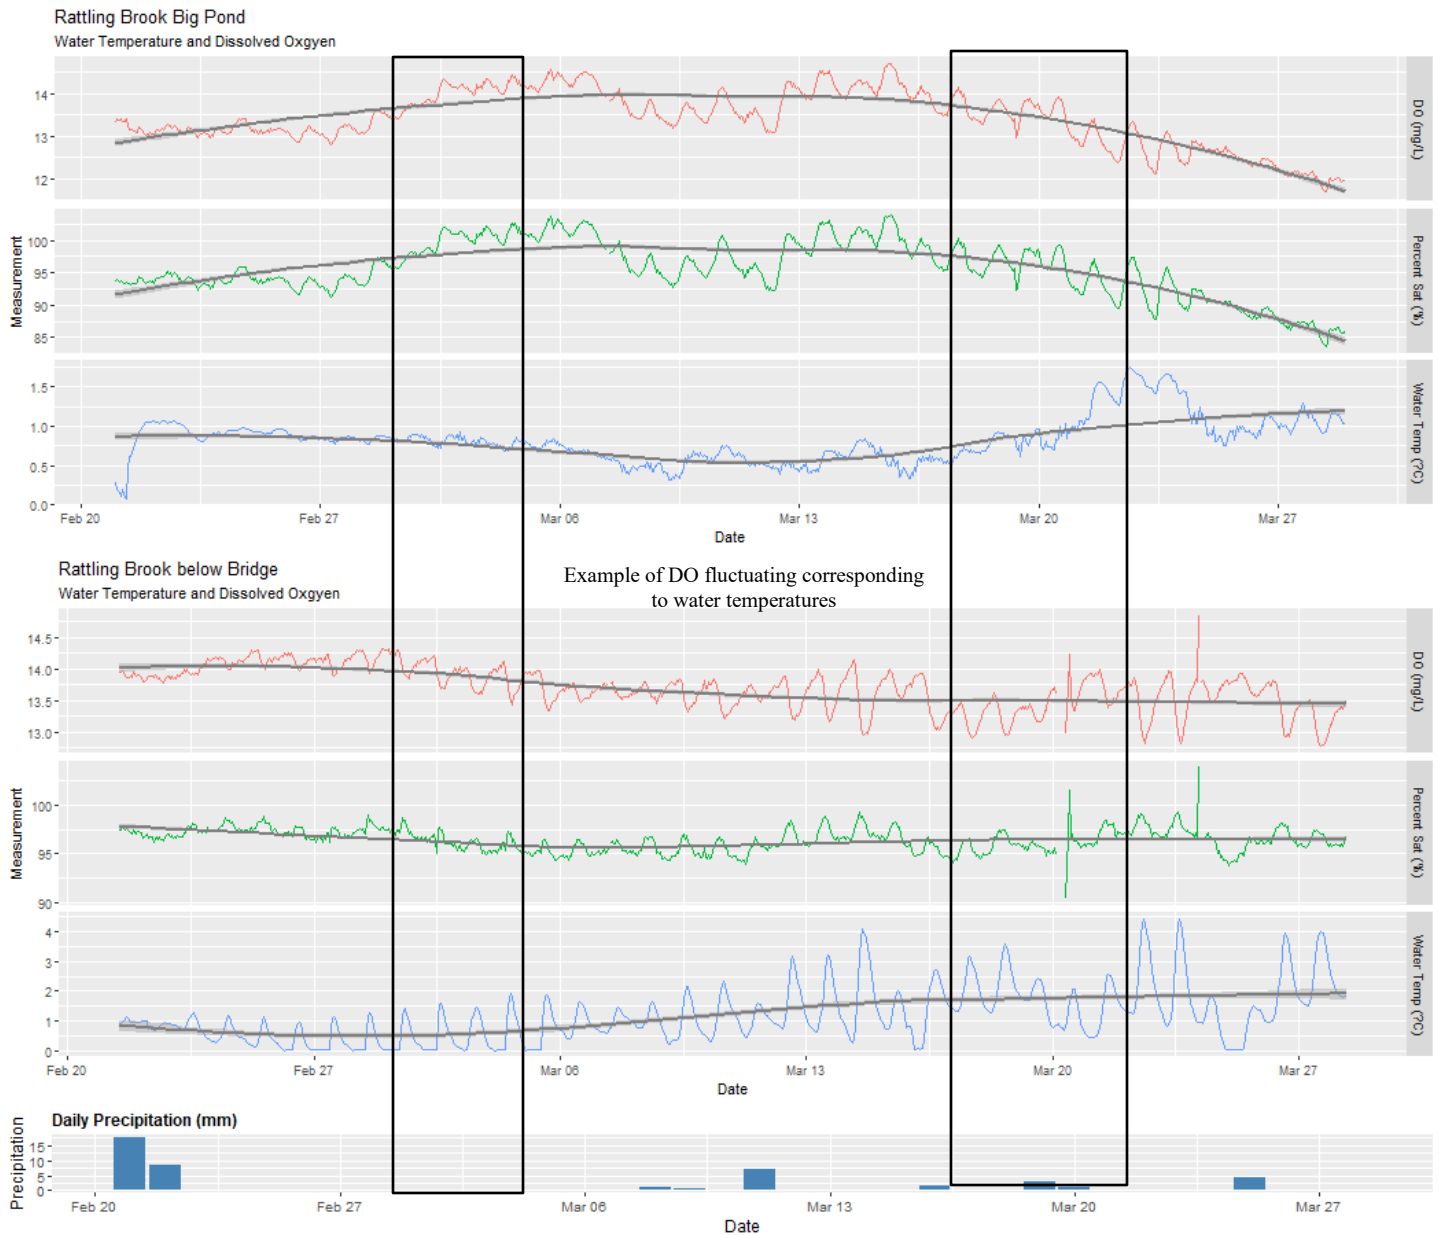

*All hydrometric data is provisional and is subject to correction. Please consult Water survey of Canada for finalized data and interpretation.

Rattling Brook Network, Long Harbour, Newfoundland and Labrador

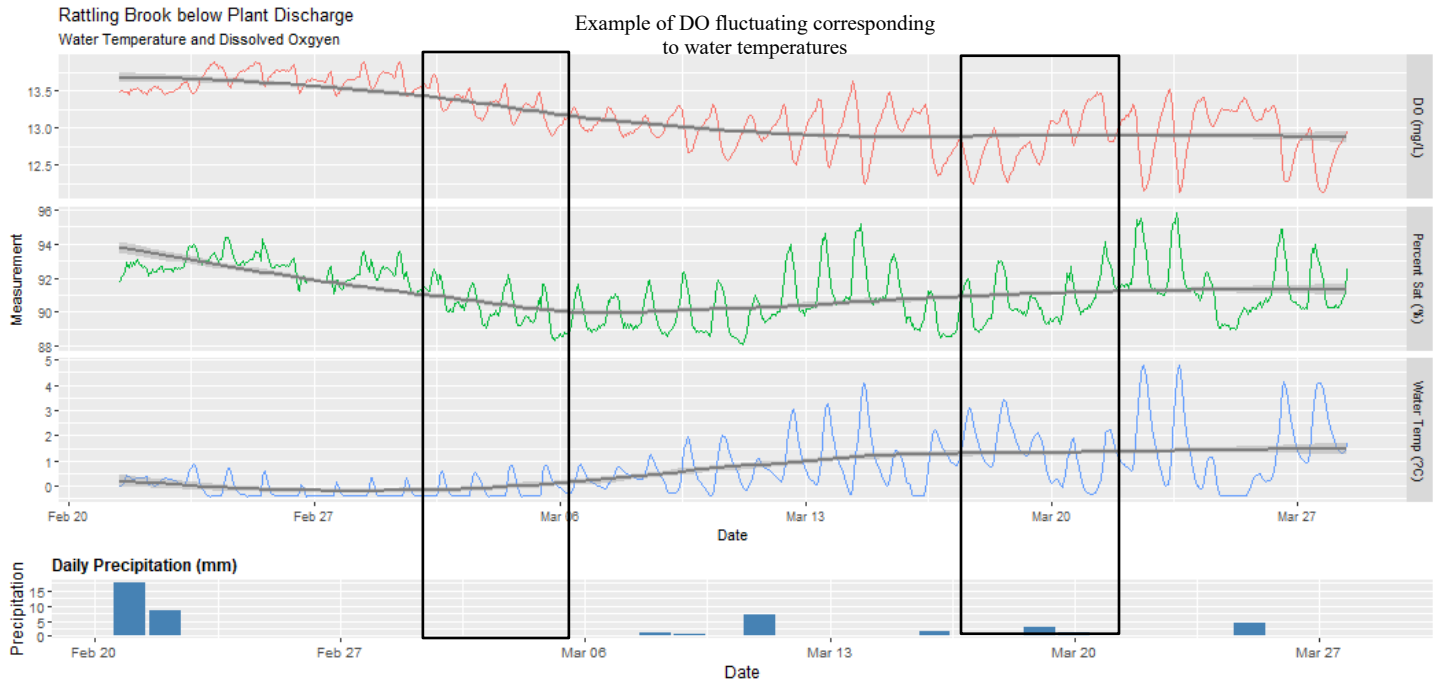


Station	Max	Min	Median	Mean
Big Pond	14.70	11.69	13.42	13.41
Below Bridge	14.85	12.77	13.73	13.70
Below Plant Discharge	13.90	12.13	13.18	13.15

- During this deployment period, all values remained above the CCME Guideline of 9.5 mg/L for the protection of early life stage cold-water biota. Trend lines show decreasing DO as water temperature warms.

*All hydrometric data is provisional and is subject to correction. Please consult Water survey of Canada for finalized data and interpretation.

Turbidity

Turbidity is typically caused by fine suspended solids such as silt, clay, or organic material. Consistently high levels of turbidity tend to block sunlight penetration into a waterbody, discouraging plant growth. High turbidity can also damage the delicate respiratory organs of aquatic animals and cover spawning areas.

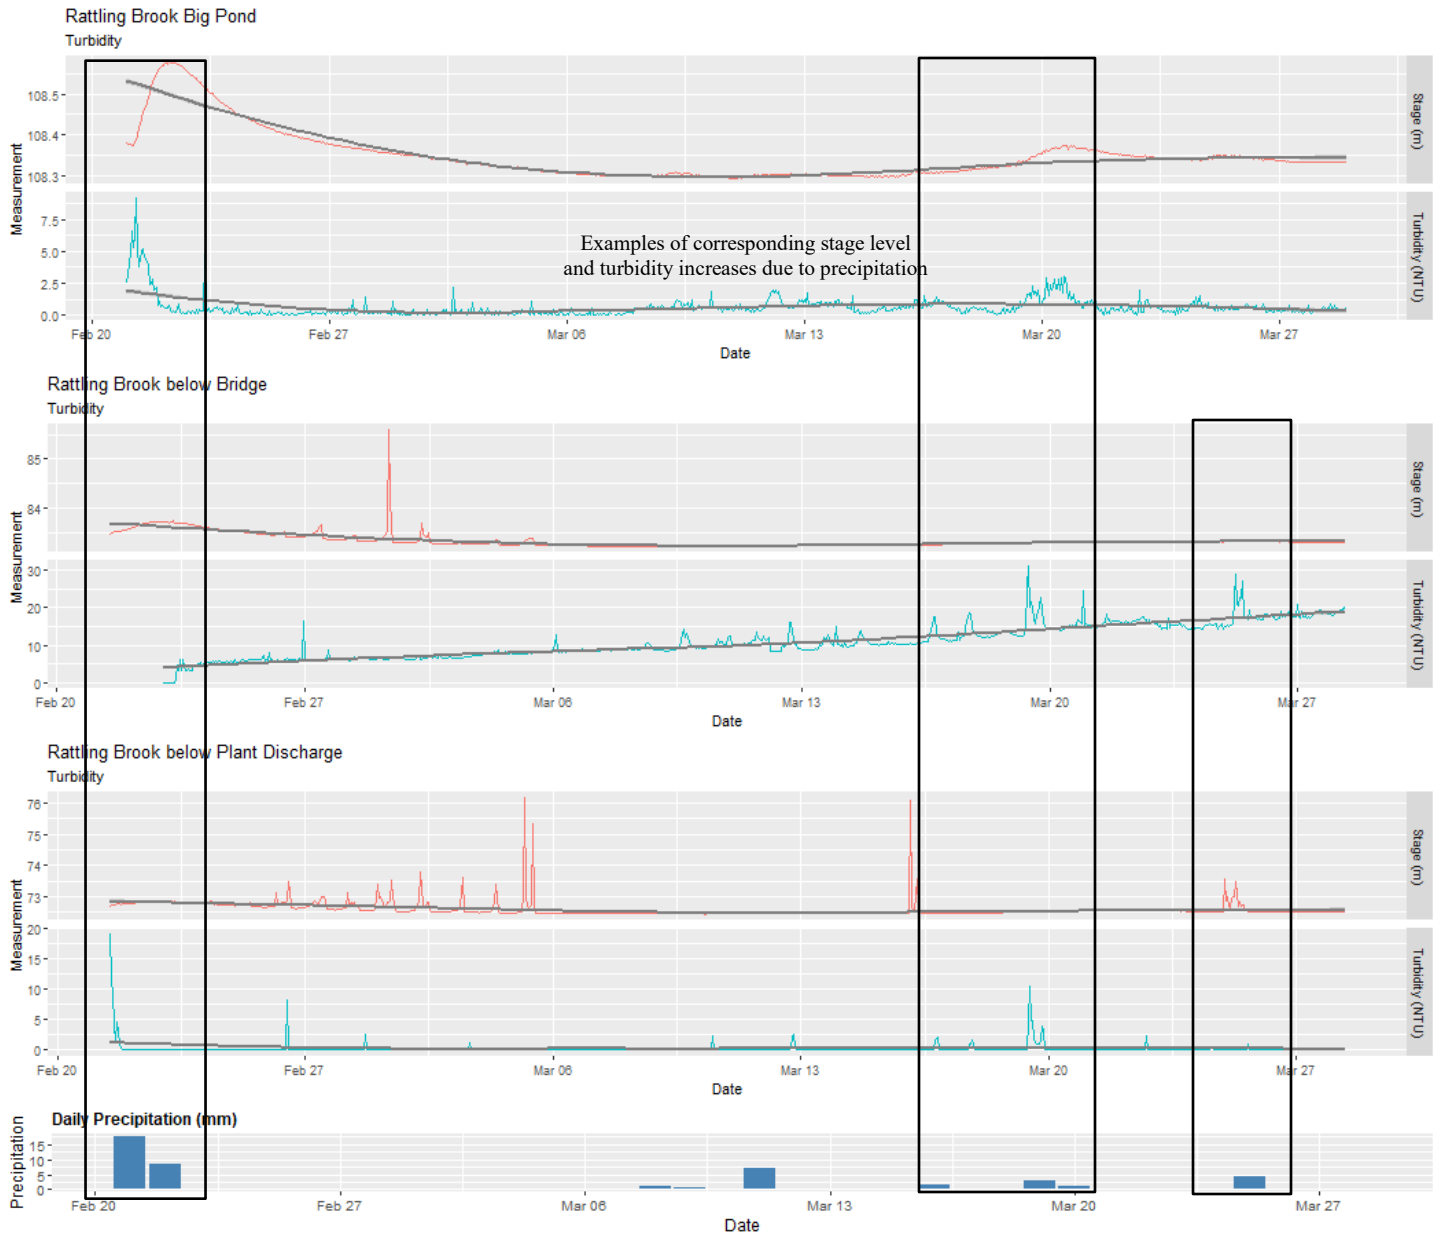

Station	Max	Min	Median	Mean
Big Pond	9.2	0.0	0.4	0.6
Below Bridge	31.0	0.0	9.6	10.5
Below Plant Discharge	19.1	0.0	0.0	0.1

- Isolated turbidity events were experienced simultaneously with precipitation events and are of short duration.

*All hydrometric data is provisional and is subject to correction. Please consult Water survey of Canada for finalized data and interpretation.

- Below Bridge experienced a gradual increase in Turbidity. During sonde removal for maintenance and calibration, it was noted that sediment encased the Turbidity sensor. This accounts for the 'poor' QAQC ranking between the field and QAQC sonde upon removal on March 28th.

Appendix

