



# Real Time Water Quality Report Teck Duck Pond Operations

Deployment Period 2015-08-04 to 2015-09-01

2015-09-24



Government of Newfoundland & Labrador  
Department of Environment and  
Conservation  
Water Resources Management Division

## General

- Water Resources Management Division (WRMD) staff monitors the real-time web page on a daily basis. Any unusual observations are investigated, with site visits being carried out as warranted.
- Management at Teck Duck Pond Operations are informed of any significant water quality events or instrumentation problems by WRMD.
- There was discharge of effluent from Polishing Pond into the receiving waters (Tributary to Gills Pond Brook) for the entire deployment period.

## Maintenance and Calibration of Instrumentation

- DataSonde**<sup>®</sup> (s/n 43245) was deployed in Tributary to Gills Pond Brook on August 4, 2015 after being cleaned and freshly calibrated, and remained deployed continuously until September 1, 2015; a 27 day period.
- DataSonde**<sup>®</sup> (s/n 43794) was deployed in East Pond Brook on August 4, 2015 after being cleaned and freshly calibrated, and remained deployed continuously until September 1, 2015; a 27 day period.
- MiniSonde**<sup>®</sup> (s/n 47591) was used for QA/QC purposes during the installation of the instruments. This unit, having the same technical specifications as the **DataSondes**<sup>®</sup>, was cleaned and freshly calibrated prior to each use.
- Quanta G**<sup>®</sup> (s/n 00035) was deployed on June 16, 2015 and remained deployed until past the end of the current reporting period.

## Quality Assurance / Quality Control (QA/QC) Measures

- As part of the QA/QC protocol, an assessment of the reliability of data recorded by an instrument is made at the beginning and end of the deployment period. The procedure is based on the approach used by the United States Geological Survey. See **Table 1**.

Parameter	Rank				
	Excellent	Good	Fair	Marginal	Poor
Temperature (oC)	<=+/-0.2	>+/-0.2 to 0.5	>+/-0.5 to 0.8	>+/-0.8 to 1	<+/-1
pH (unit)	<=+/-0.2	>+/-0.2 to 0.5	>+/-0.5 to 0.8	>+/-0.8 to 1	>+/-1
Sp. Conductance (µS/cm)	<=+/-3	>+/-3 to 10	>+/-10 to 15	>+/-15 to 20	>+/-20
Sp. Conductance > 35 µS/cm (%)	<=+/-3	>+/-3 to 10	>+/-10 to 15	>+/-15 to 20	>+/-20
Dissolved Oxygen (mg/L) (% Sat)	<=+/-0.3	>+/-0.3 to 0.5	>+/-0.5 to 0.8	>+/-0.8 to 1	>+/-1
Turbidity <40 NTU (NTU)	<=+/-2	>+/-2 to 5	>+/-5 to 8	>+/-8 to 10	>+/-10
Turbidity > 40 NTU (%)	<=+/-5	>+/-5 to 10	>+/-10 to 15	>+/-15 to 20	>+/-20

**Table 1**

- For the Surface Water Stations, upon deployment and removal, a QA/QC **MiniSonde**<sup>®</sup> is usually temporarily deployed along side the Field **DataSonde**<sup>®</sup>. Values for each recorded parameter are compared between the two instruments. Based upon the difference between the parameters recorded by the Field **DataSonde**<sup>®</sup> and QA/QC **MiniSonde**<sup>®</sup> a qualitative statement (Ranking) is usually made on the data.
- The rankings at the beginning and end of the deployment period are shown in **Table 2** for Tributary to Gill's Pond Brook and **Table 3** for East Pond Brook. There are no rankings for Well After Tailings Dam (MW1) as the instrument was neither deployed nor removed during this reporting period.

- A 'Poor' ranking was calculated for specific conductance upon removal from Tributary to Gills Pond Brook. It is noted that part way through the deployment period following a period of rainfall and increased stage, specific conductance values were lower than anticipated, and the characteristic of the graph much more variable. There was a difference of 497 ( $\mu\text{S}/\text{cm}$ ) or 50% between the Sonde that was deployed in the field versus a QA/QC instrument. However, subsequent bench testing of this instrument in the lab following its removal, confirmed that the instrument was calibrated appropriately and providing accurate readings over a wide range of conductivity standards. Accordingly, the data has been left in the data set.
- A 'Poor' ranking was calculated for Temperature upon deployment in East Pond Brook. There was a difference of 1.84 °C, over water temperatures which were near 25 °C.
- Because the deployment set-up for Well After Tailings Dam (MW1) is different, comparison with another instrument is not possible. In this case, a grab sample is usually collected at the beginning and end of the deployment period, and the ranking is calculated for pH and Specific Conductivity based upon live data and laboratory data.
- As **Quanta G**<sup>®</sup> (s/n 00035) was deployed in this well, prior to the beginning of this reporting period, the ranking for the initial deployment is documented in a previous report. As the unit remains deployed, rankings for removal will be documented in a subsequent report.
- With the exception of water quantity data (Stage and Flow), all data used in the preparation of the graphs and subsequent discussion below adhere to this stringent QA/QC protocol. Water Survey of Canada is responsible for QA/QC of water quantity data. Corrected data can be obtained upon request.

Tributary to Gills Pond Brook Station (NF02YO0190)		
Date (yyyy-mm-dd)	Parameter	Ranking
2015-08-04 Installation	Temp (°C)	Excellent
	pH (units)	Excellent
	Sp. Conductivity ( $\mu\text{S}/\text{cm}$ )	Excellent
	Dissolved Oxygen (mg/L)	Excellent
	Turbidity (NTU)	Excellent
2015-09-01 Removal	Temp (°C)	Excellent
	pH (units)	Excellent
	Sp. Conductivity ( $\mu\text{S}/\text{cm}$ )	Poor
	Dissolved Oxygen (mg/L)	Excellent
	Turbidity (NTU)	Good

Table 2

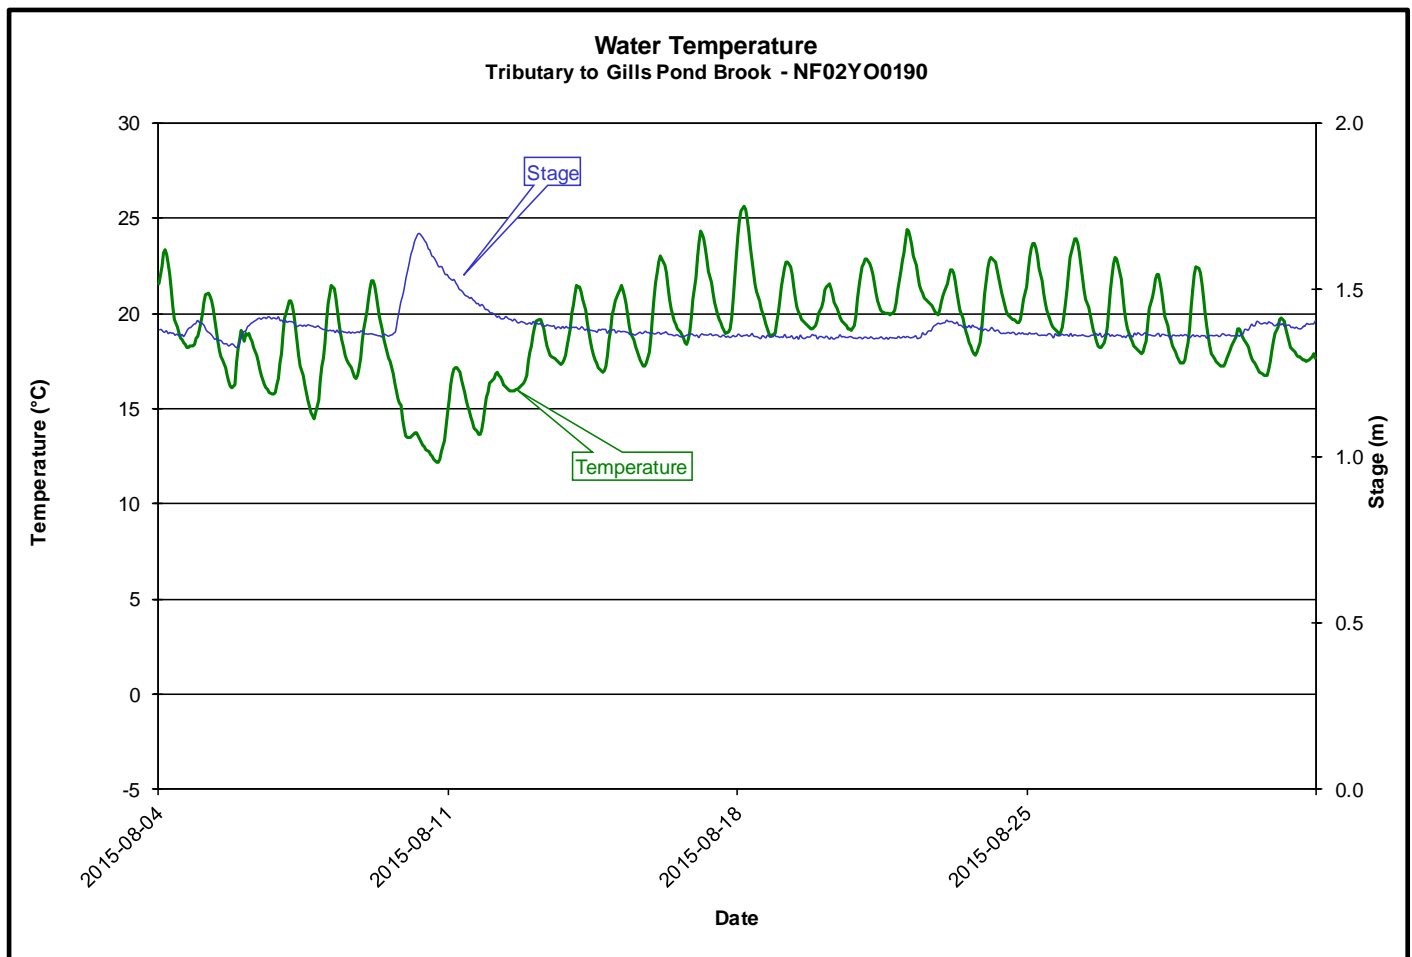
East Pond Brook Station (NF02YO0192)		
Date (yyyy-mm-dd)	Parameter	Ranking
2015-08-04 Installation	Temp (°C)	Poor
	pH (units)	Good
	Sp. Conductivity ( $\mu\text{S}/\text{cm}$ )	Excellent
	Dissolved Oxygen (mg/L)	Excellent
	Turbidity (NTU)	Excellent
2015-09-01 Removal	Temp (°C)	Excellent
	pH (units)	Excellent
	Sp. Conductivity ( $\mu\text{S}/\text{cm}$ )	Excellent
	Dissolved Oxygen (mg/L)	Excellent
	Turbidity (NTU)	Excellent

Table 3

## Data Interpretation

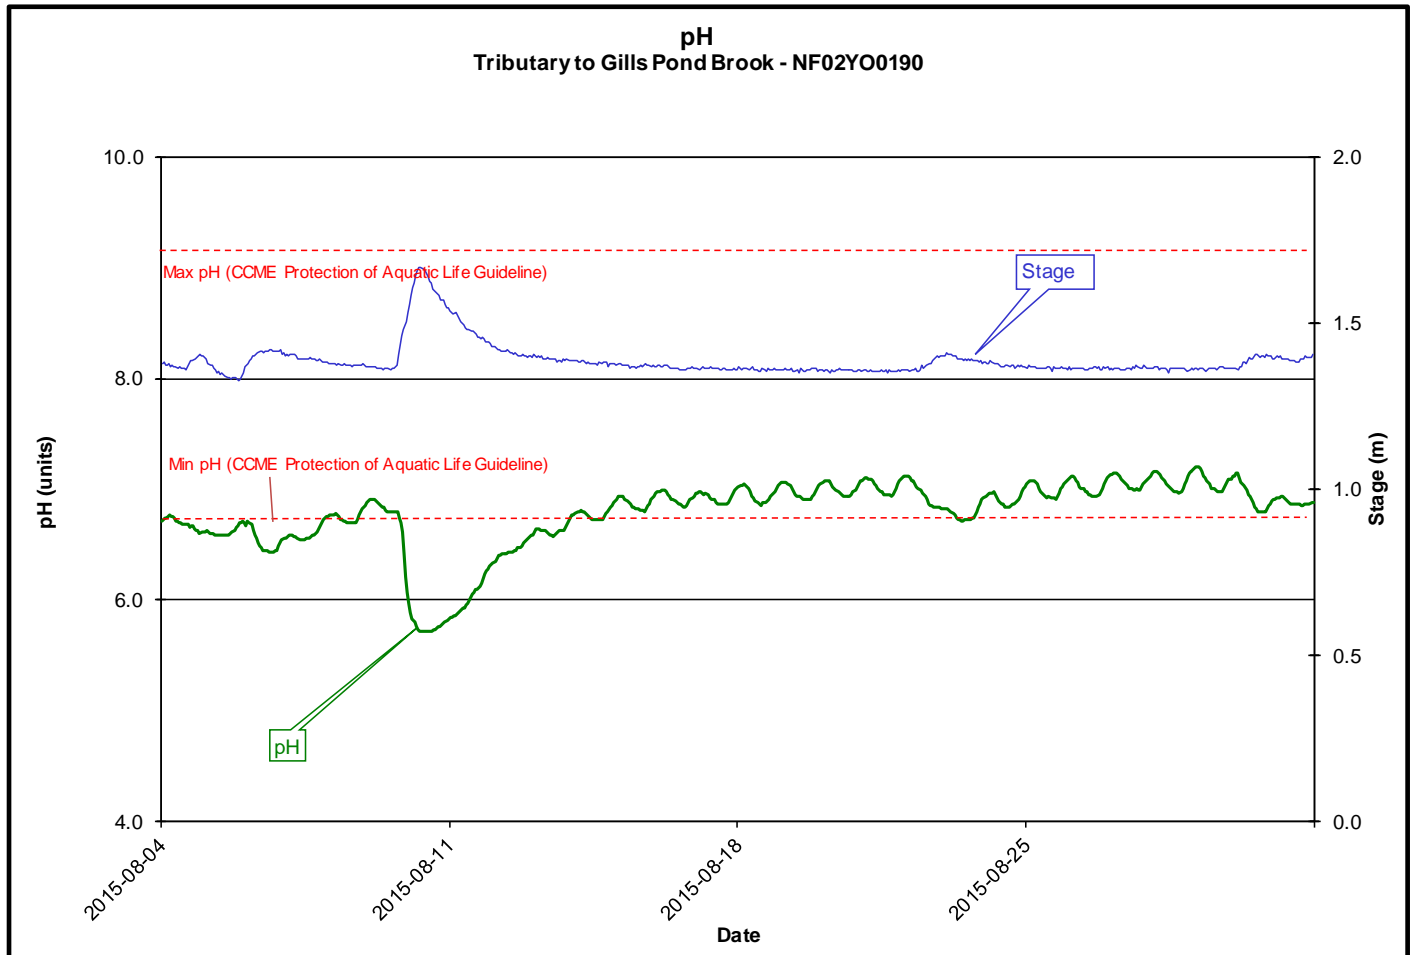
### TRIBUTARY TO GILLS POND BROOK

- The water temperature (**Figure 1**) ranged from a minimum of 12.17°C to a maximum of 25.62°C.
- Water temperatures were slightly lower, with less diurnal variation during a period of increased stage during this deployment period.

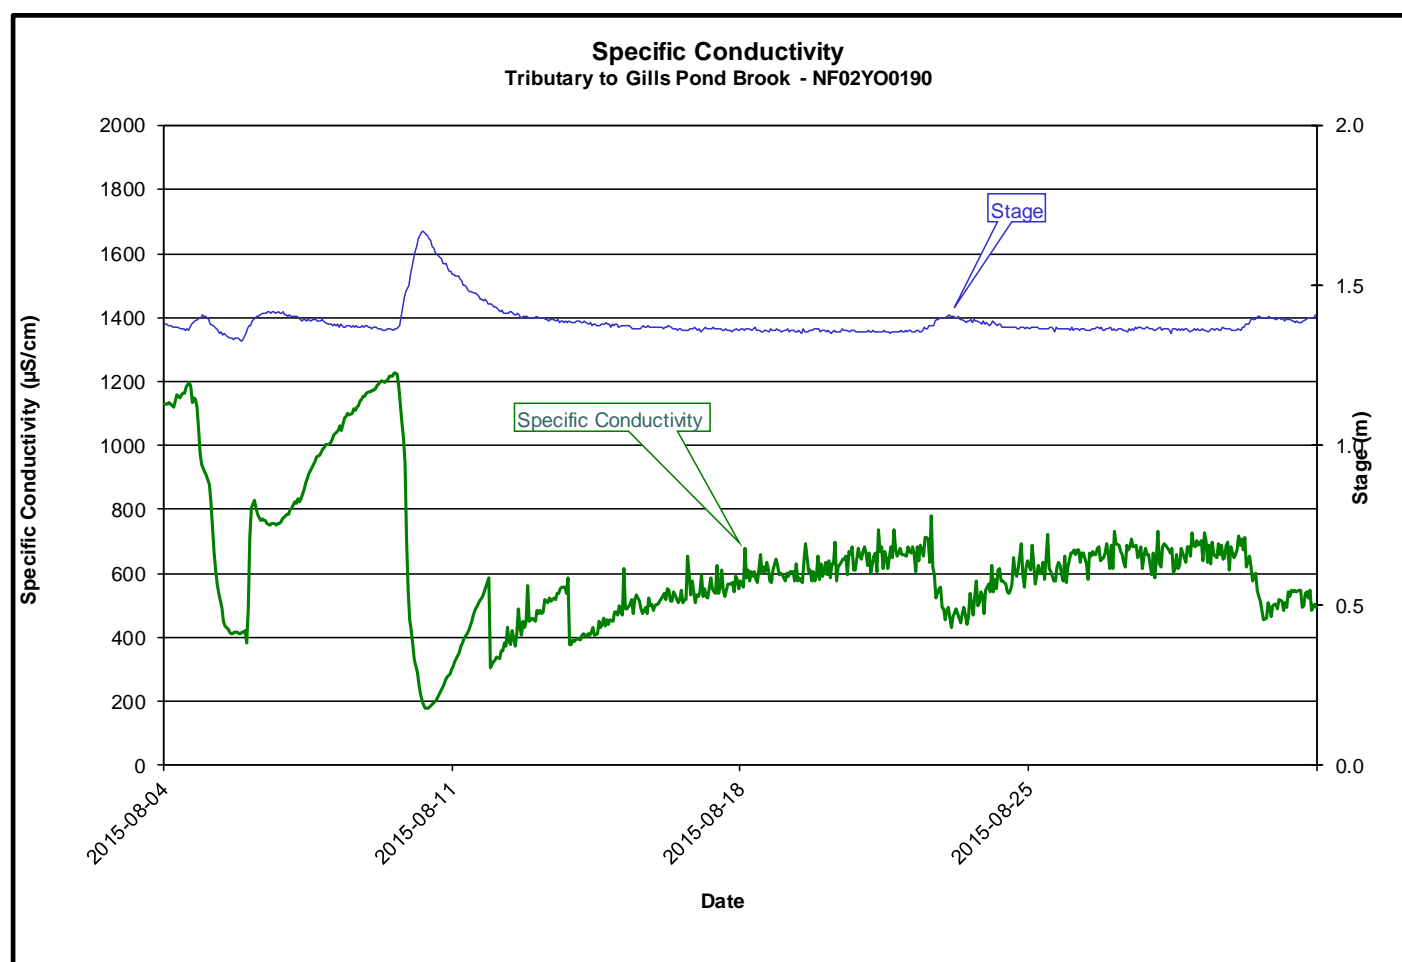


**Figure 1**

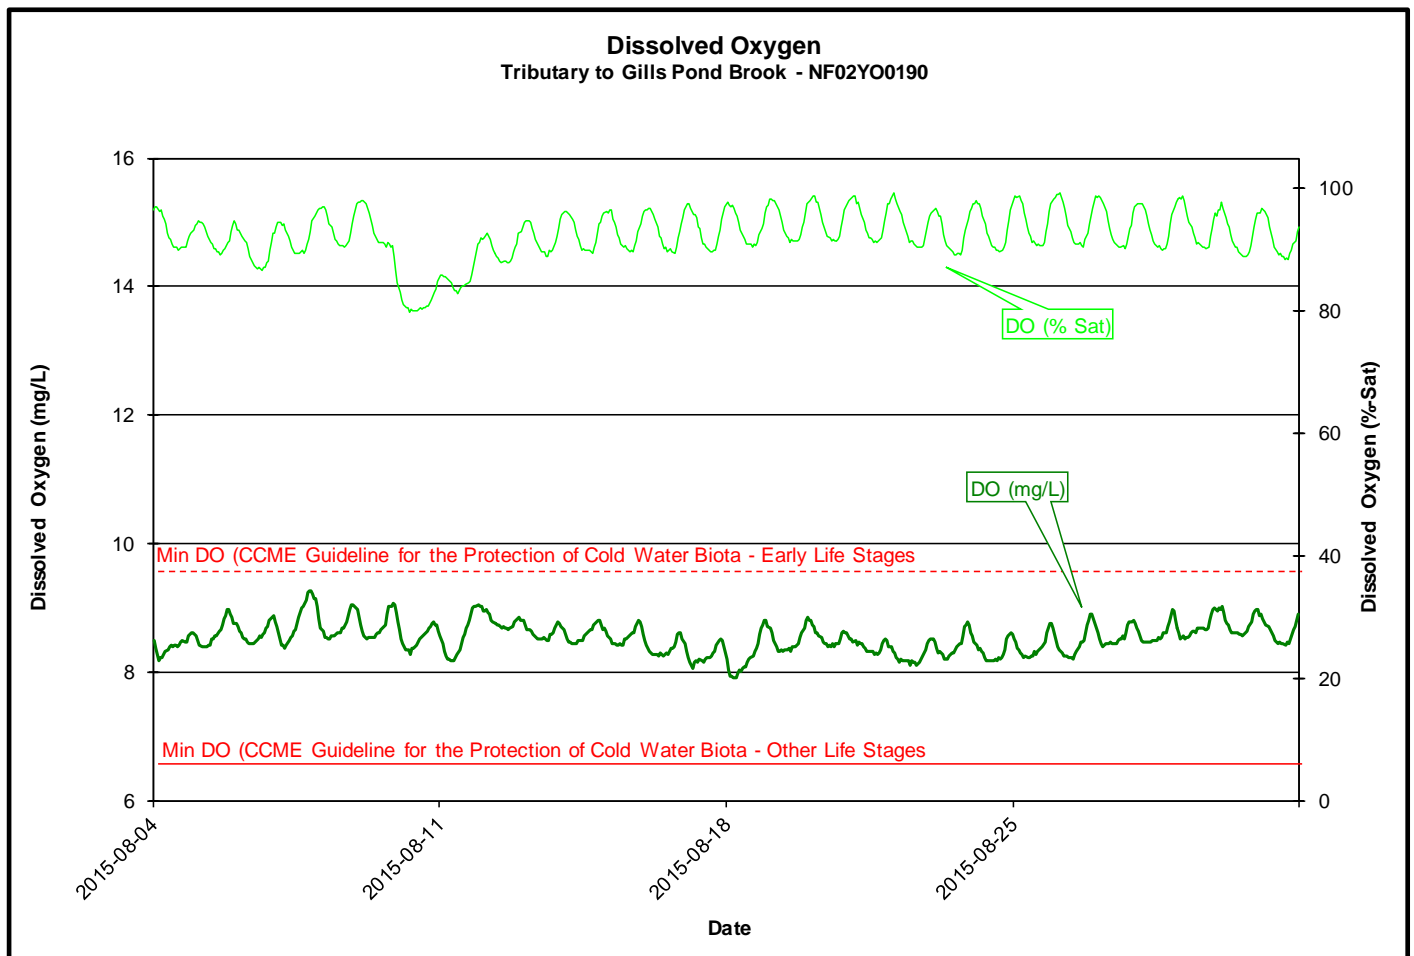
- Throughout the deployment period, pH values (**Figure 2**) ranged from a minimum of 5.71 to a maximum of 7.20.
- During this deployment period pH remained near the lower limit of the recommended range (6.5 – 9.0) for the CCME *Canadian Water Quality Guidelines for the Protection of Aquatic Life*.
- An inverse relationship with stage is obvious throughout the deployment period.

**Figure 2**

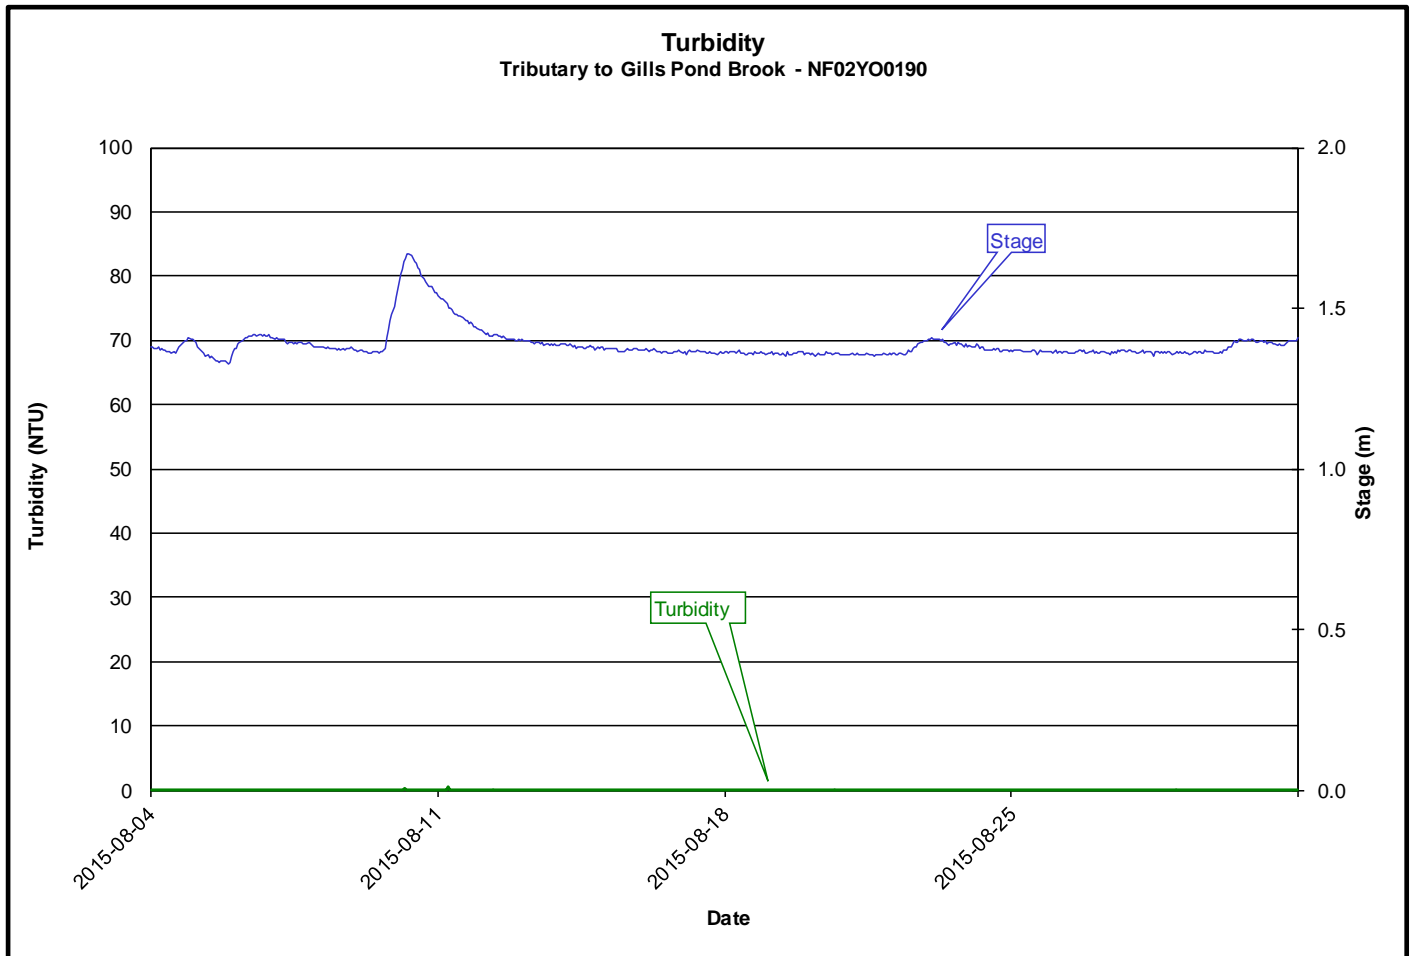
- The specific conductivity (**Figure 3**) ranged from a minimum of 175.6  $\mu\text{S}/\text{cm}$  to a maximum of 1228.0  $\mu\text{S}/\text{cm}$  over the deployment period.
- It is noted that part way through the deployment period following a period of rainfall and increased stage, specific conductance values were lower than anticipated, and the characteristic of the graph much more variable. At the end of the deployment period, there was a difference of 497 ( $\mu\text{S}/\text{cm}$ ) or 50% between the Sonde that was deployed in the field versus a QA/QC instrument. However, subsequent bench testing of this instrument in the lab following its removal, confirmed that the instrument was calibrated appropriately and providing accurate readings over a wide range of conductivity standards. Accordingly, the data has been left in the data set.
- There is an inverse relationship between specific conductivity and stage, highlighted over several instances over this deployment period. This is essentially the dilution effect of the rainwater on the highly conductive discharge water.

**Figure 3**

- The dissolved oxygen (**Figure 4**) values ranged from a minimum of 7.91 mg/L to a maximum of 9.27 mg/L over the deployment period, with the percent saturation ranging between 79.7 and 99.4.
- Dissolved oxygen (mg/L) levels are fairly consistent across the deployment period.
- All of the dissolved oxygen values fell above the minimum for Other Life Stages (CCME *Canadian Water Quality Guidelines for the Protection of Aquatic Life* cold water/other life stages – above 6.5 mg/L; cold water/early life stages – above 9.5 mg/L). This range is typical based upon water temperatures.
- Based upon the fact that dissolved oxygen % saturation had minimal and predictable change over the deployment period, we can be confident that the dissolved oxygen mg/L values are accurate.

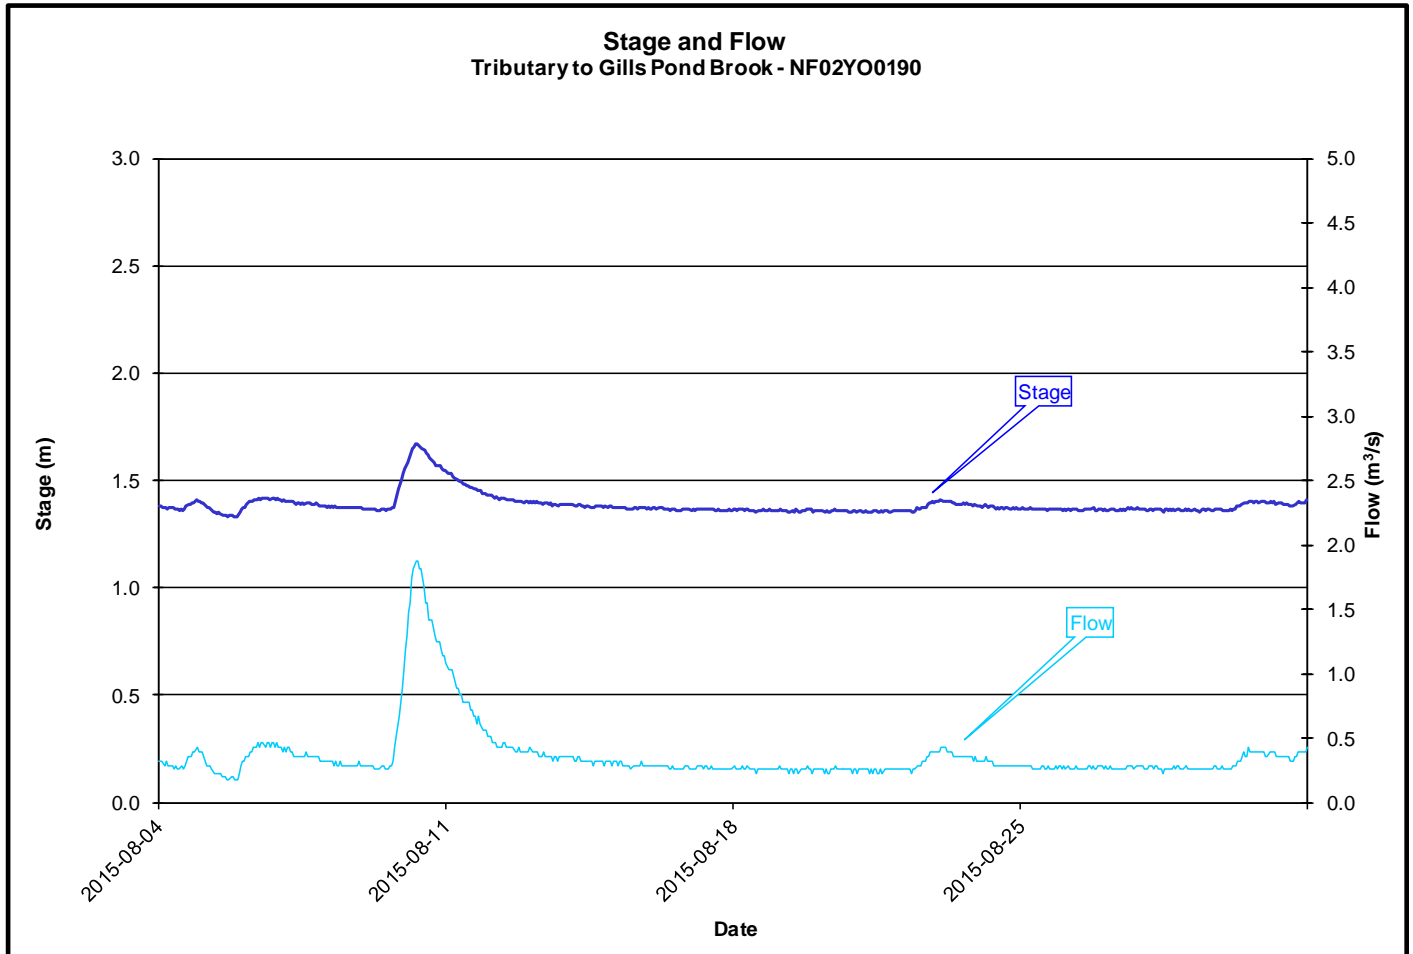
**Figure 4**

- The turbidity values (**Figure 5**) ranged from a minimum of 0.0 NTU to a maximum of 0.6 NTU.
- No issues with turbidity were evident.

**Figure 5**

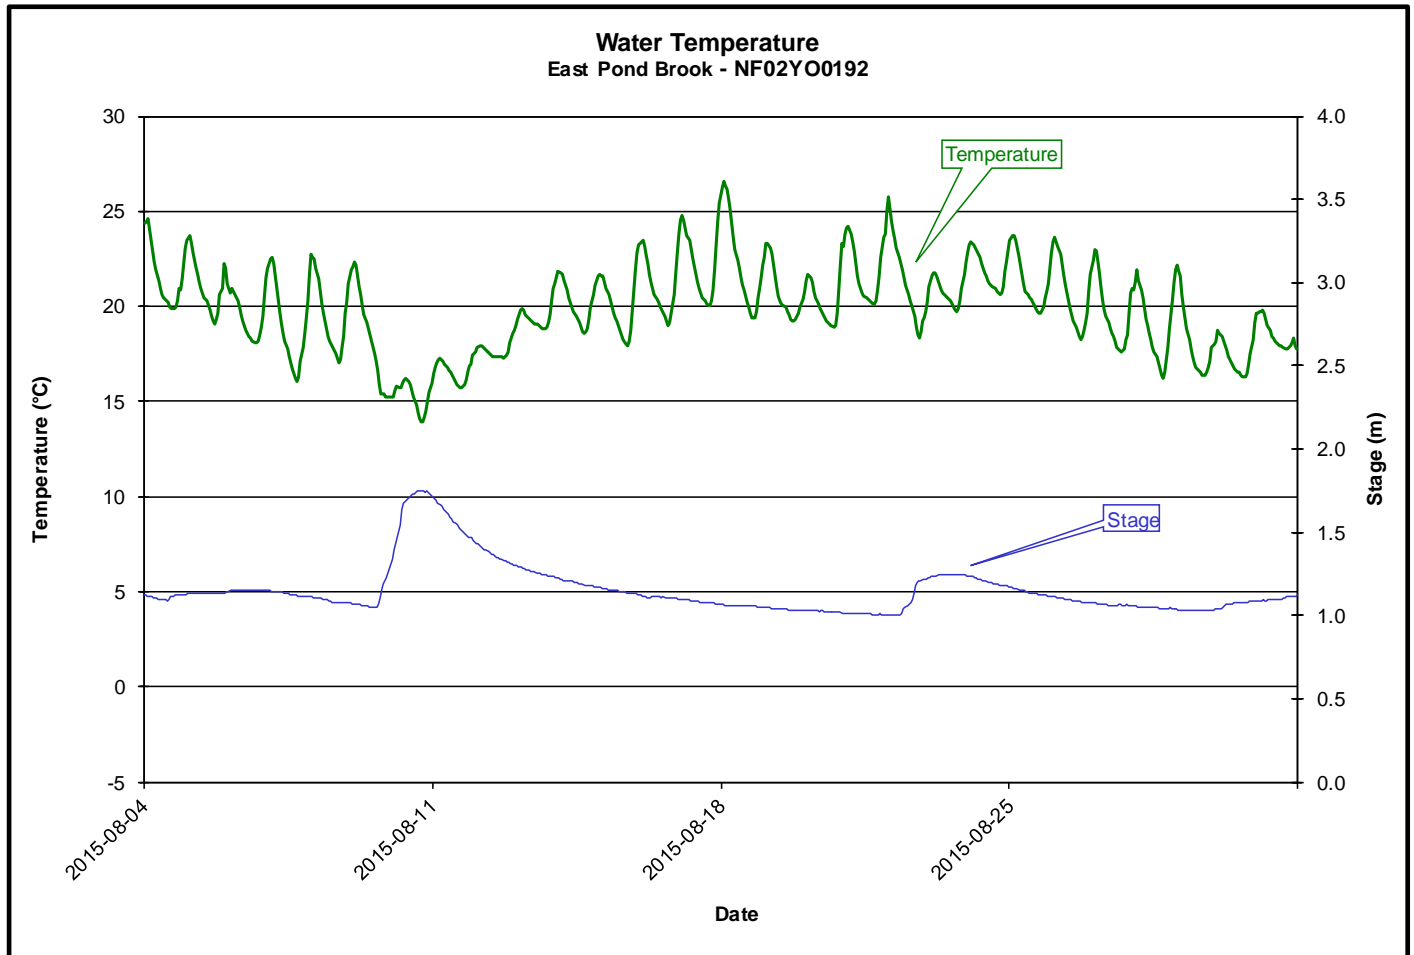


- The stage or water level ranged from a minimum of 1.33 m to a maximum of 1.67 m. The flow or discharge ranged from a minimum of 0.18 m<sup>3</sup>/s to a maximum of 1.88 m<sup>3</sup>/s (**Figure 6**).
- Increases in stage and flow are the result of precipitation/runoff events.
- Stage and flow are all within normal ranges.
- Water Survey of Canada is responsible for QA/QC of water quantity data. Corrected data can be obtained upon request.

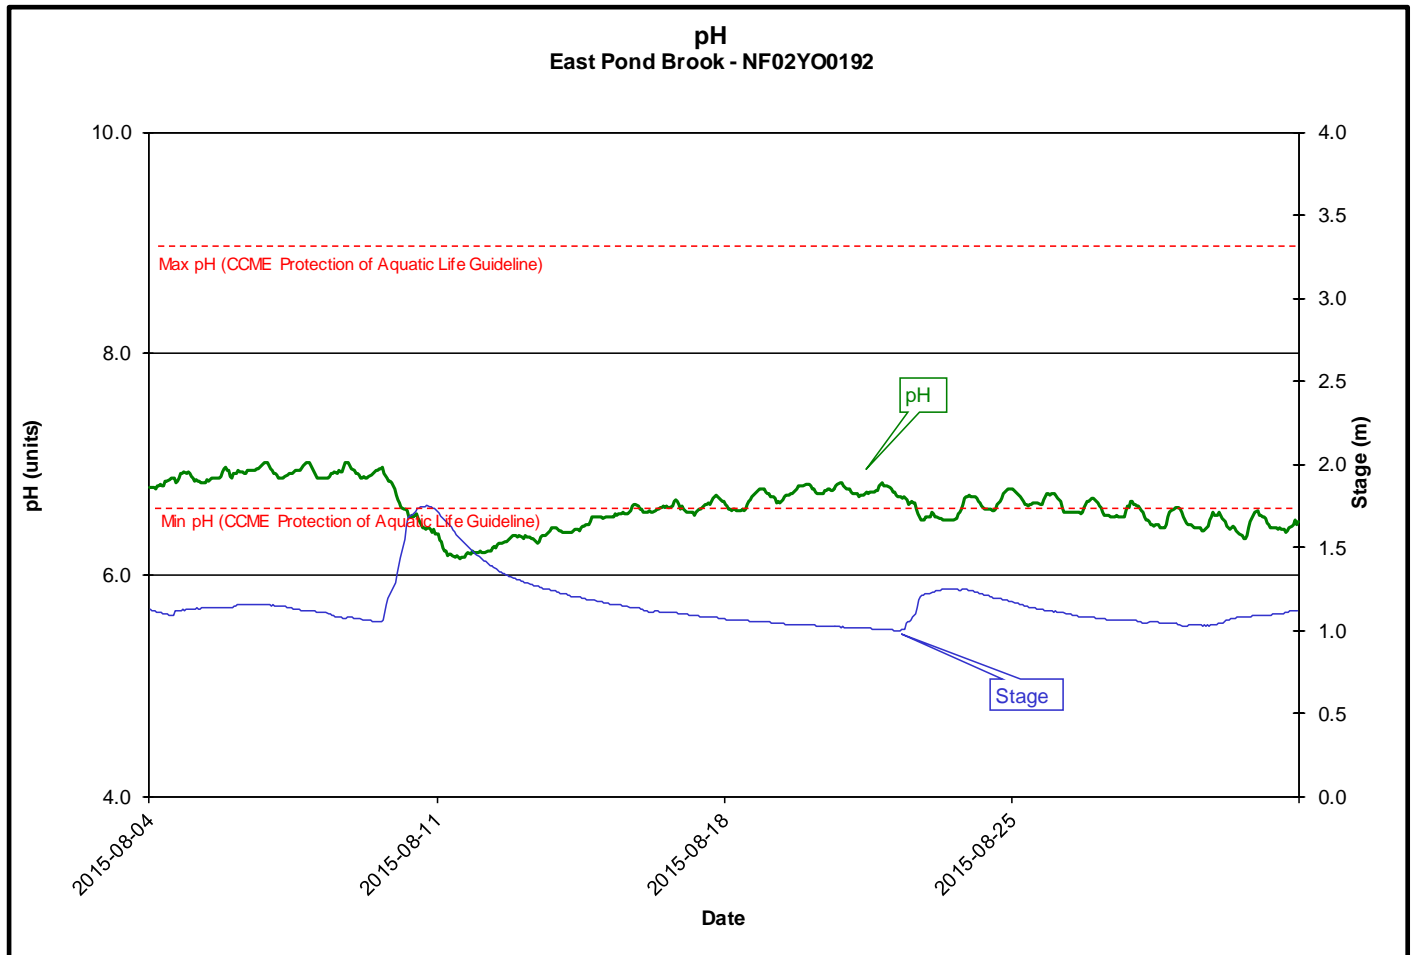
**Figure 6**

**EAST POND BROOK**

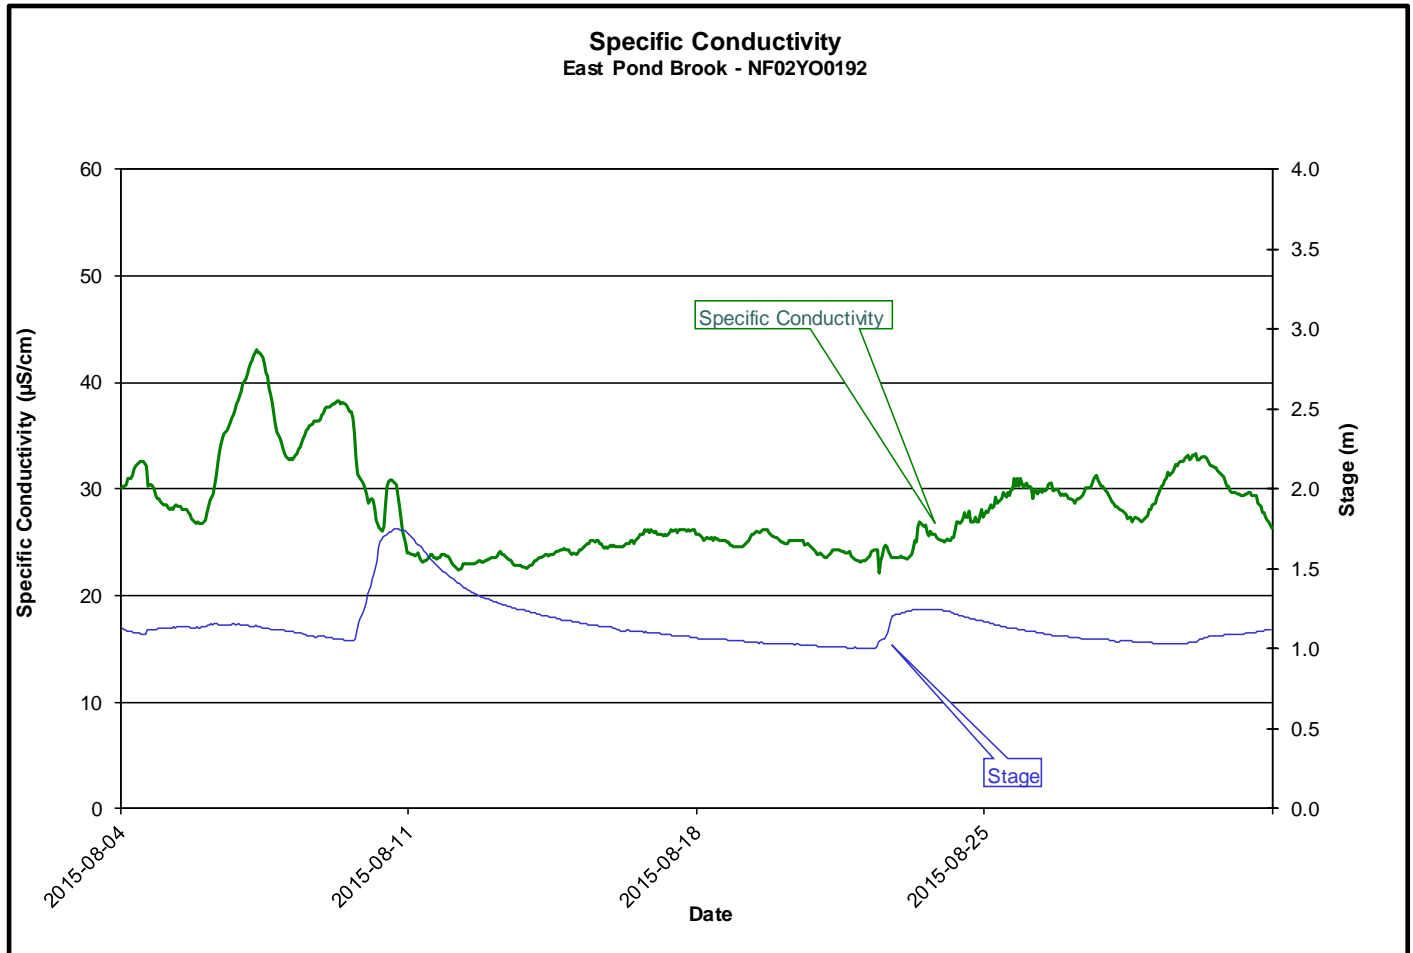
- The water temperature (**Figure 7**) ranged from a minimum of 13.93 °C to a maximum of 26.60 °C.
- Water temperatures remained fairly constant over the deployment period.
- There does not appear to be any correlation with stage during this deployment period, however there is less diurnal variation during a period of higher stage.

**Figure 7**

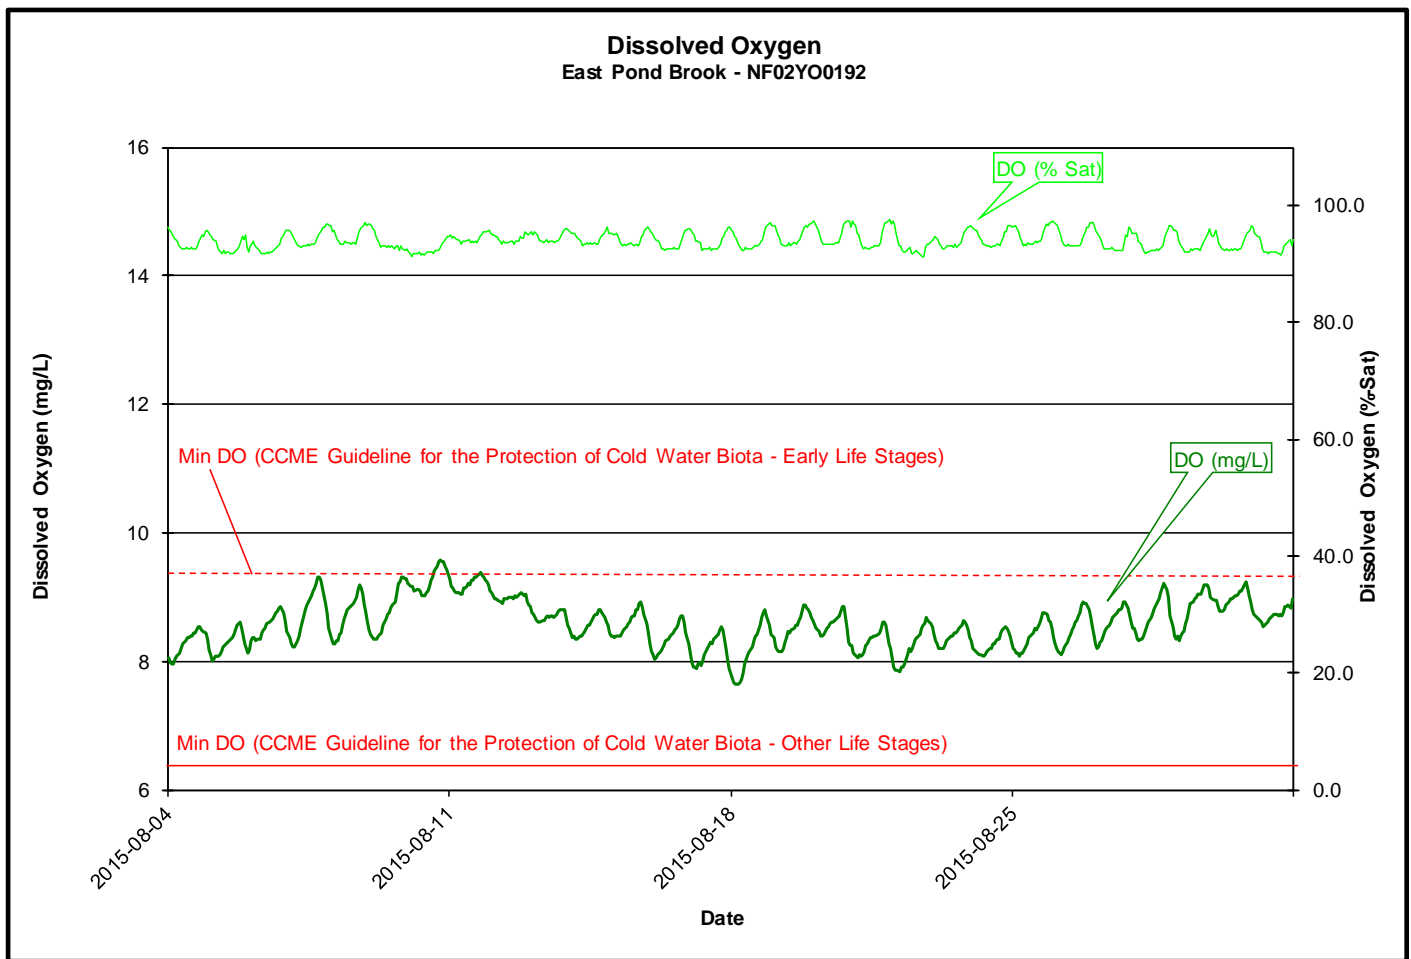
- Throughout the deployment period pH values (**Figure 8**) ranged from a minimum of 6.15 to a maximum of 7.02.
- Throughout the deployment period, pH values were right around the lower limit of the recommended range (6.5 – 9.0) for the CCME *Canadian Water Quality Guidelines for the Protection of Aquatic Life*.
- There is an inverse relationship between pH and stage evident during this deployment period.
- The background pH of this stream is normally quite low, and values near and below the lower limit are not unusual.

**Figure 8**

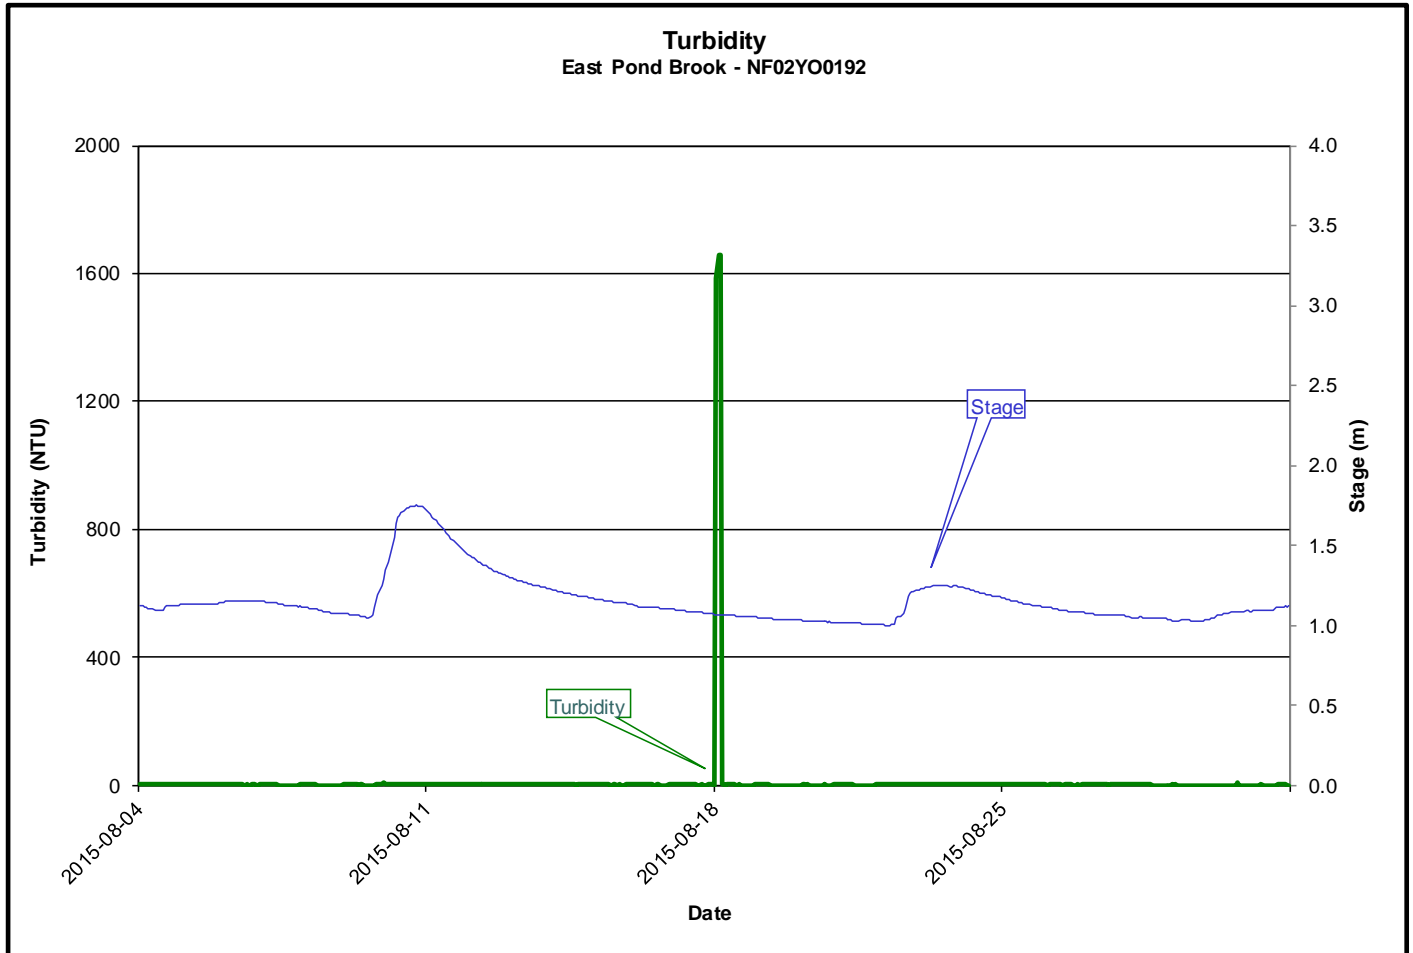
- The specific conductivity (**Figure 9**) ranged from a minimum of 22.1  $\mu\text{S}/\text{cm}$  to a maximum of 43.0  $\mu\text{S}/\text{cm}$ .
- Conductivity values in this range are typical for this stream.

**Figure 9**

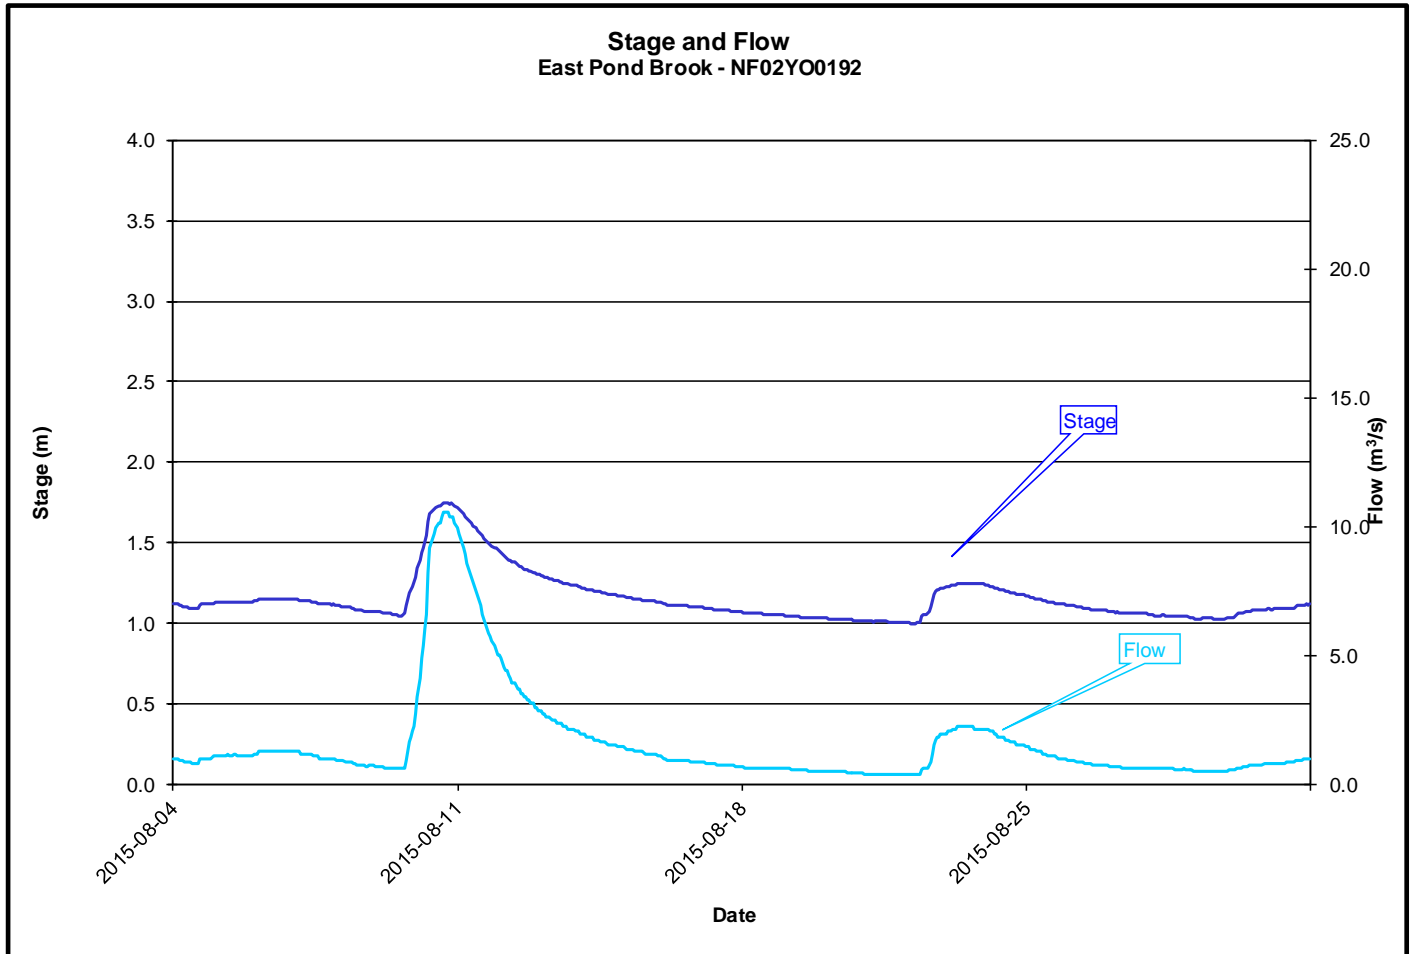
- The dissolved oxygen (**Figure 10**) values ranged from a minimum of 7.64 mg/L to a maximum of 9.57 mg/L over the deployment period, with the percent saturation ranging between 91.3 and 97.6.
- Dissolved oxygen (mg/L) levels are fairly consistent across the deployment period.
- All of the dissolved oxygen values fell above the minimum for Other Life Stages (CCME *Canadian Water Quality Guidelines for the Protection of Aquatic Life* cold water/other life stages – above 6.5 mg/L; cold water/early life stages – above 9.5 mg/L). This range is typical based upon water temperatures.
- Based upon the fact that dissolved oxygen % saturation had minimal and predictable change over the deployment period, we can be confident that the dissolved oxygen mg/L values are accurate.

**Figure 10**

- The turbidity values (**Figure 11**) ranged from a minimum of 0.0 NTU to a maximum of 1660.0 NTU.
- The one major and short duration spike in turbidity is likely the result of natural in-stream debris passing near the sensor.
- Very low turbidity values are typical in this stream.

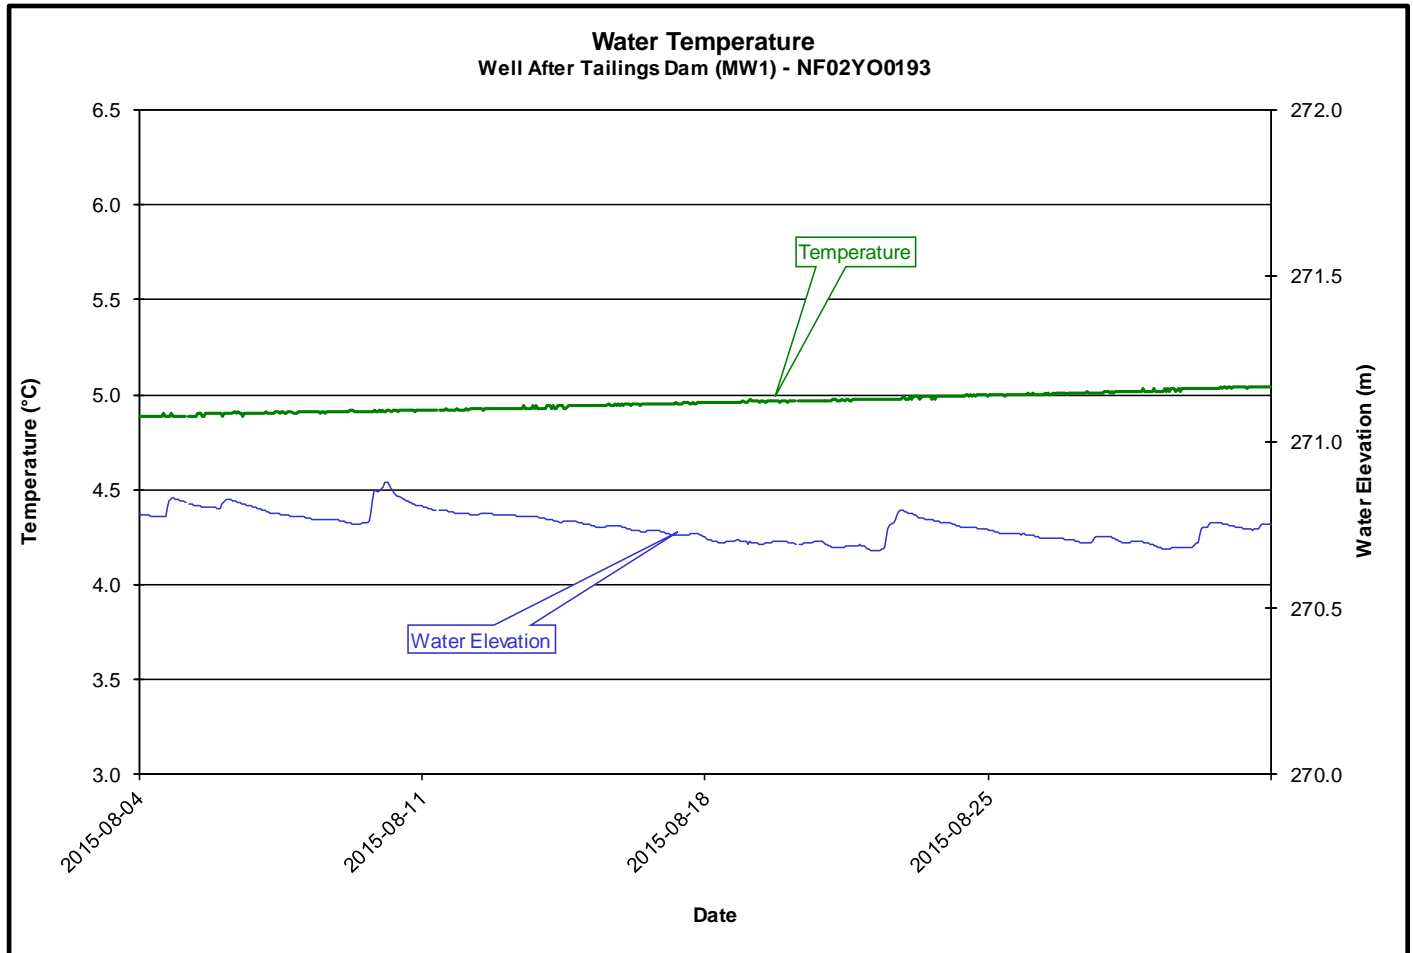
**Figure 11**

- The stage or water level ranged from a minimum of 1.00 m to a maximum of 1.75 m. The flow or discharge ranged from a minimum of 0.37 m<sup>3</sup>/s to a maximum of 10.56 m<sup>3</sup>/s (**Figure 12**).
- Increase in stage and flow are the result of precipitation/runoff events.
- Stage and flow are all within normal ranges.
- Water Survey of Canada is responsible for QA/QC of water quantity data. Corrected data can be obtained upon request.

**Figure 12**

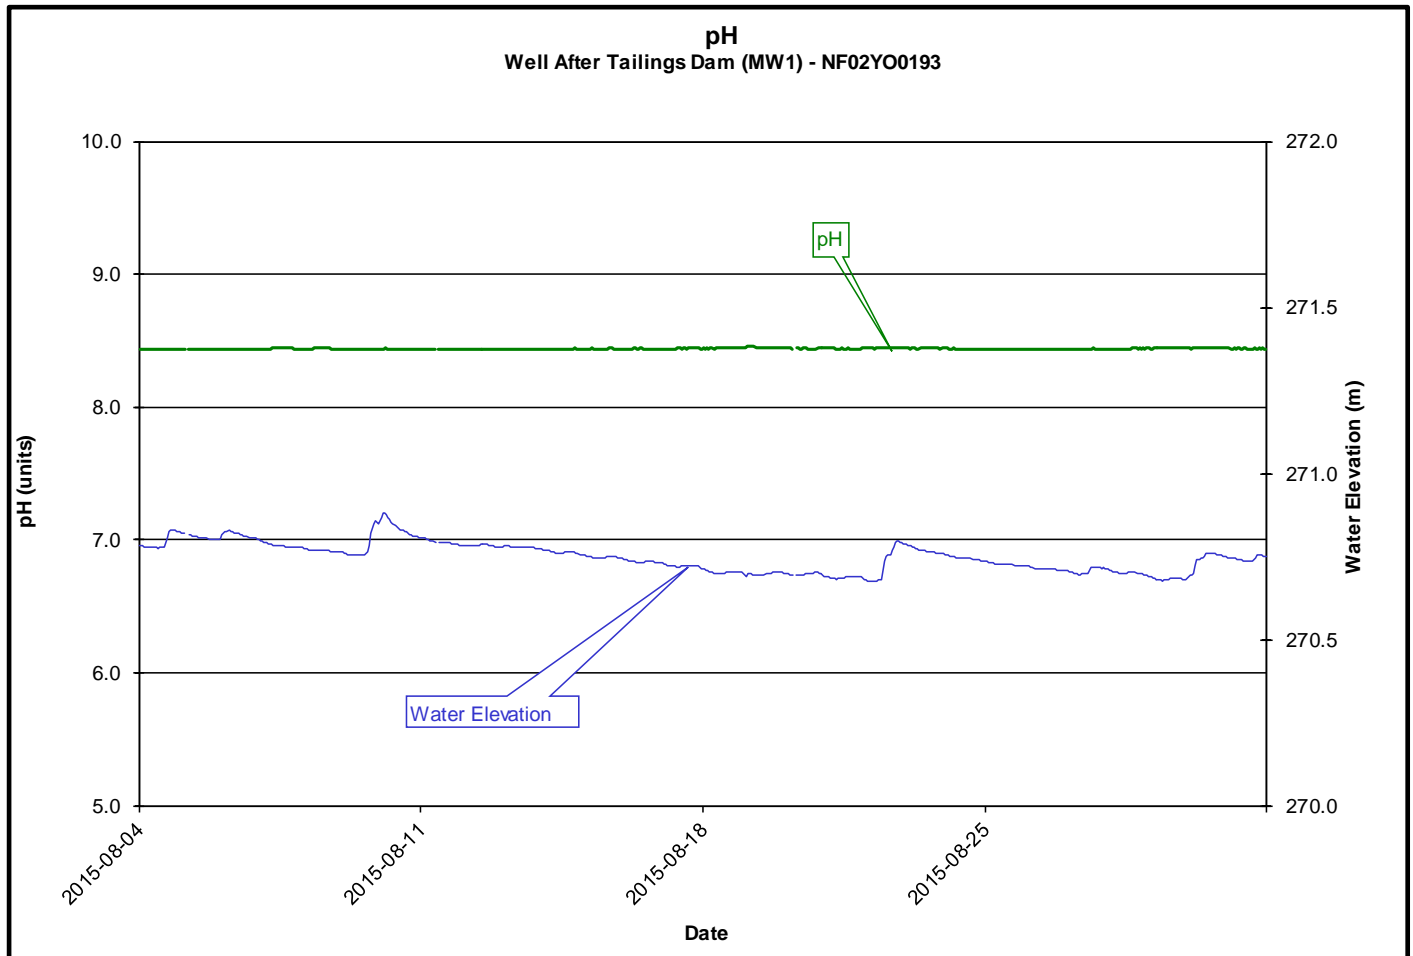
**WELL AFTER TAILING DAM (MW1)**

- The water temperature (**Figure 13**) ranged from a minimum of 4.89 °C to a maximum of 5.04 °C with a slight increase over the reporting period.
- There appears to be no correlation with water elevation.

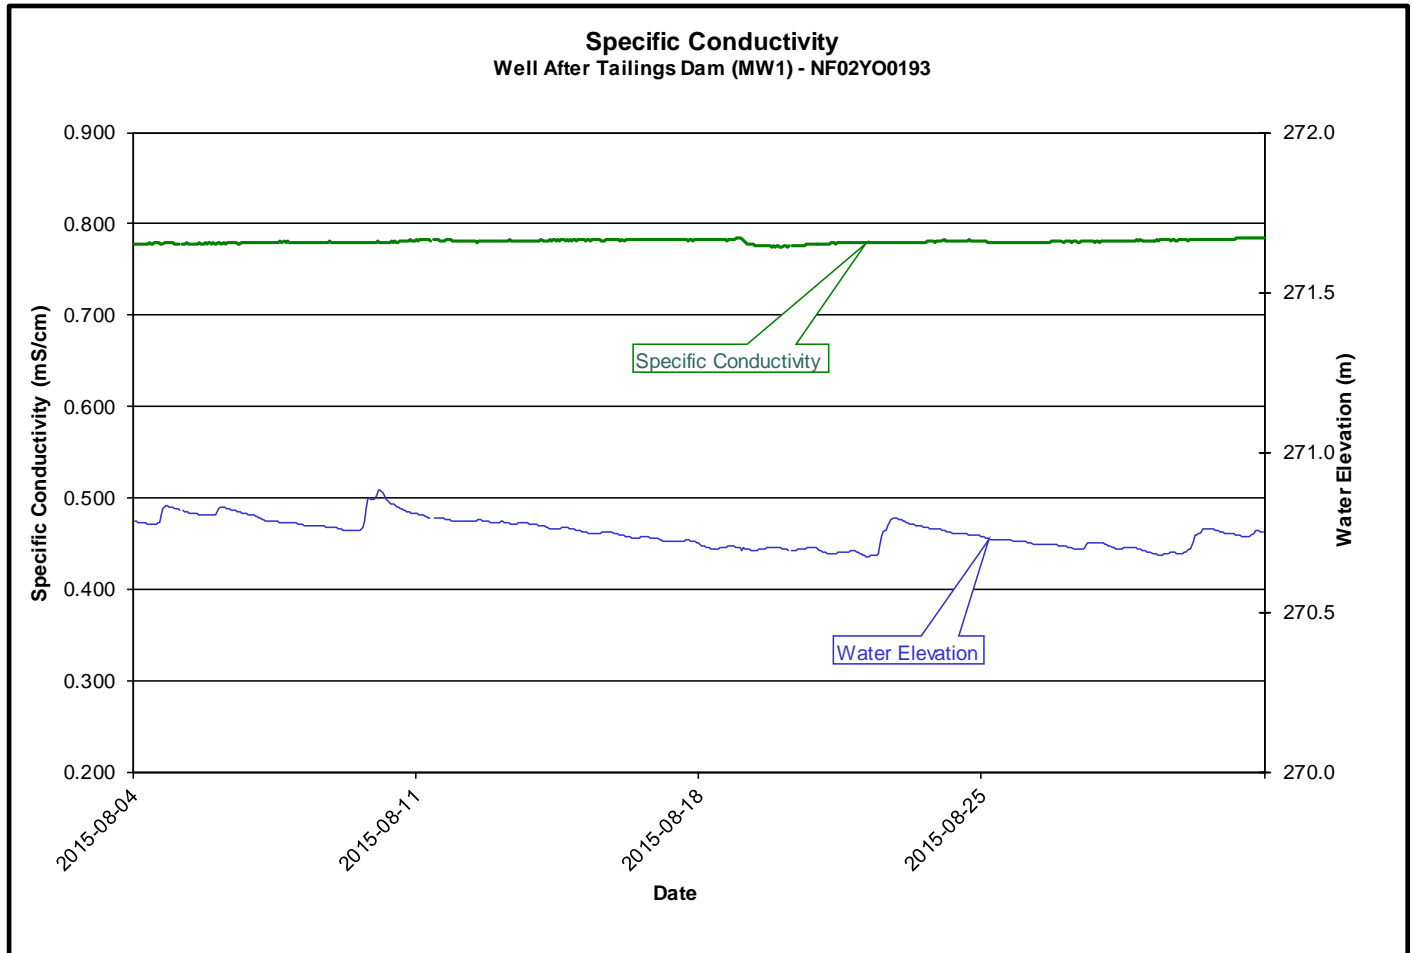
**Figure 13**



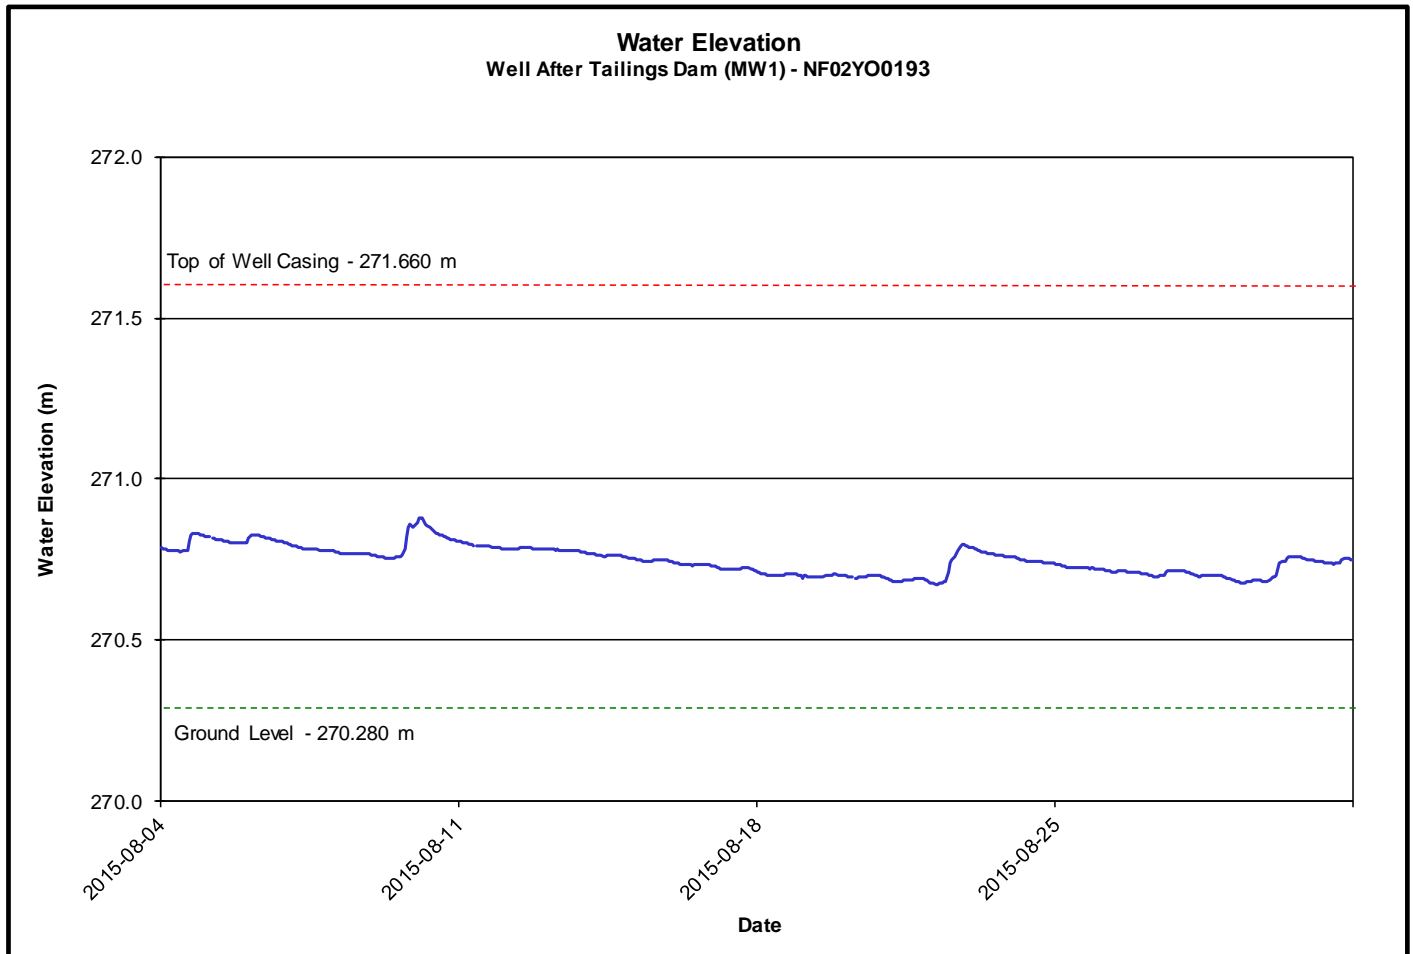
- The pH (**Figure 14**) ranged from a minimum of 8.44 to a maximum of 8.46.
- There was little change in pH over the deployment period.
- There does not appear to be any correlation with water elevation.

**Figure 14**

- The specific conductivity (**Figure 15**) ranged from a minimum of 0.775 mS/cm to a maximum of 0.785 mS/cm.
- There was little change over the reporting period.

**Figure 15**

- The Water Elevation (**Figure 16**) ranged from a minimum of 270.67 m to a maximum of 270.88 m.
- Water elevation in this well corresponds to increased water level in an adjacent stream, and is influenced by precipitation/runoff events, as well as the water elevation in the nearby Tailings Management Area.



**Figure 16**

Prepared by:

Robert Wight  
Environmental Scientist  
Water Resources Management Division  
Department of Environment and Conservation  
Tel: 709-292-4280  
Fax: 709-292-4365  
e-mail: [robertwight@gov.nl.ca](mailto:robertwight@gov.nl.ca)